PACSmate®

PACSmate Technology Inc.

MODEL:

POC-17i/19i Series

Medical Panel PC with Intel® Core™ i7/i5/i3 Processor, TFT LCD, Wireless LAN, Touch Screen, RS-232/422/485 and RoHS

User Manual

Rev. 1.00 – 7 August, 2013

RoHS Lead Free

Revision

Date	Version	Changes
7 August, 2013	1.00	Initial release

Copyright

COPYRIGHT NOTICE

The information in this document is subject to change without prior notice in order to improve reliability, design and function and does not represent a commitment on the part of the manufacturer.

In no event will the manufacturer be liable for direct, indirect, special, incidental, or consequential damages arising out of the use or inability to use the product or documentation, even if advised of the possibility of such damages.

This document contains proprietary information protected by copyright. All rights are reserved. No part of this manual may be reproduced by any mechanical, electronic, or other means in any form without prior written permission of the manufacturer.

TRADEMARKS

All registered trademarks and product names mentioned herein are used for identification purposes only and may be trademarks and/or registered trademarks of their respective owners.

Contact Information

Headquarters

IEI Integration Corp.
Address: No. 29, Zongxing Rd., Xizhi Dist.,
New Taipei City 221, Taiwan
Phone: +886-2-8691-6798
Fax: +886-2-6616-0028
Web Site: www.ieiworld.com
Sales Email: sales@ieiworld.com.tw

USA

IEI Integration USA Corp.
Address: 138 University Parkway,
Pomona, CA 91768
Phone: +1-909-595-2819
Fax: +1-909-595-2816
Web Site: www.ieiworld.com
Sales Email: sales@usa.ieiworld.com.tw

Table of Contents

1 INTRODUCTION 1

1.1 OVERVIEW 2
1.2 FEATURES 3
1.3 EXTERNAL OVERVIEW 3
1.3.1 General Description 3
1.3.2 Front Panel 3
1.3.3 Rear Panel 4
1.3.4 I/O Interface Panel 5
1.3.5 OSD Control Buttons 6
1.4 INTERNAL OVERVIEW 6
1.5 SYSTEM SPECIFICATIONS 7
1.6 DIMENSIONS 9

2 UNPACKING 11

2.1 UNPACKING 12
2.2 PACKING LIST 13

3 INSTALLATION 15

3.1 ANTI-STATIC PRECAUTIONS 16
3.2 INSTALLATION PRECAUTIONS 16
3.3 INSTALLATION AND CONFIGURATION STEPS 17
3.4 REMOVING THE REAR PANEL COVER 17
3.5 REMOVING THE INTERNAL ALUMINUM COVER 18
3.6 JUMPER SETTINGS 19
3.6.1 Access the Jumpers 20
3.6.2 Preconfigured Jumpers 20
3.6.3 Clear CMOS Jumper 21
3.6.4 COM1 Pin 9 Setting 22
3.6.5 COM3 TX Function Select Jumper 24
3.6.6 COM3 RS-232/422/485 Jumper 25

3.6.6.1 COM3 RS-422 and RS-485 Pinouts 26
3.6.7 COM3 RS Function Select Jumper 27
3.6.8 ME Debug Mode Jumper 28
3.6.9 iTPM Setting Jumper 29
3.6.10 ME RTC Select Jumper 30
3.6.11 SPI Setting Jumper 31
3.7 MOUNTING THE SYSTEM 32
3.7.1 Wall Mounting 32
3.7.2 Arm Mounting 35
3.8 BOTTOM PANEL CONNECTORS 37
3.8.1 LAN Connection 37
3.8.2 Serial Device Connection 38
3.8.3 USB Device Connection 38
3.8.4 VGA Monitor Connection 39
3.9 AT/ATX MODE SELECTION 40
3.9.1 AT Power Mode 41
3.9.2 ATX Power Mode 41

4 SYSTEM MAINTENANCE 42

4.1 SYSTEM MAINTENANCE INTRODUCTION 43
4.2 ANTI-STATIC PRECAUTIONS 43
4.3 TURN OFF THE POWER 44
4.4 REPLACING COMPONENTS 44
4.4.1 Memory Module Replacement 44
4.4.2 HDD Card Replacement 46

5 BIOS SETUP 49

5.1 INTRODUCTION 50
5.1.1 Starting Setup 50
5.1.2 Using Setup 50
5.1.3 Getting Help 51
5.1.4 Unable to Reboot After Configuration Changes 51
5.1.5 BIOS Menu Bar 51
5.2 MAIN 52
5.3 ADVANCED 53

5.3.1 ACPI Settings *54*
5.3.2 Trusted Computing *55*
5.3.3 CPU Configuration *56*
5.3.4 SATA Configuration *57*
5.3.5 USB Configuration *58*
5.3.6 Super IO Configuration *59*
5.3.6.1 Serial Port n Configuration 60
5.3.7 H/W Monitor *64*
5.3.8 Serial Port Console Redirection *65*
5.4 CHIPSET 66
5.4.1 Northbridge Configuration *67*
5.4.2 Southbridge Configuration *68*
5.4.3 Intel IGD SWSCI OpRegion *69*
5.5 BOOT 71
5.6 SECURITY 72
5.7 EXIT 73

6 SOFTWARE DRIVERS 75

6.1 AVAILABLE SOFTWARE DRIVERS 76
6.2 CHIPSET DRIVER INSTALLATION 76
6.3 VGA DRIVER INSTALLATION 80
6.4 LAN DRIVER INSTALLATION 84
6.5 AUDIO DRIVER INSTALLATION 87
6.5.1 BIOS Setup *87*
6.5.2 Driver Installation *87*
6.6 TOUCH SCREEN DRIVER 90
6.7 WIRELESS DRIVER 93
6.8 KEYPAD DRIVER 96

A SAFETY PRECAUTIONS 101

A.1 SAFETY PRECAUTIONS 102
A.1.1 General Safety Precautions *102*
A.1.2 Explanation of Graphical Symbols *103*
A.1.3 Anti-static Precautions *104*
A.1.4 Product Disposal *105*

A.2 MAINTENANCE AND CLEANING PRECAUTIONS 105
A.2.1 Maintenance and Cleaning 105
A.2.2 Cleaning Tools 106
A.3 FCC PRECAUTIONS 106

B BIOS OPTIONS 108

B.1 BIOS CONFIGURATION OPTIONS 109

C WATCHDOG TIMER 111

D HAZARDOUS MATERIALS DISCLOSURE 114

D.1 HAZARDOUS MATERIAL DISCLOSURE TABLE FOR IPB PRODUCTS CERTIFIED AS ROHS COMPLIANT UNDER 2002/95/EC WITHOUT MERCURY 115

List of Figures

Figure 1-1: POC-17i/19i Series Medical Panel PC 2
Figure 1-2: Front View 4
Figure 1-3: Rear View 4
Figure 1-4: I/O Interface Connector Panel 5
Figure 1-5: OSD Control Buttons 6
Figure 1-6: POC-17i Series Dimensions (mm) 9
Figure 1-7: POC-17i Series Dimensions (mm) 10
Figure 3-1: Back Cover Retention Screws 18
Figure 3-2: Aluminum Back Cover Retention Screws 19
Figure 3-3: Clear CMOS Jumper 22
Figure 3-4: JP7 Jumper Setting Location 23
Figure 3-5: JP8 Jumper Setting Location 24
Figure 3-6: COM3 TX Function Select Jumper Location 25
Figure 3-7: COM3 RS-232/422/485 Serial Port Select Jumper Location 26
Figure 3-8: COM3 RX Function Select Jumper Location 28
Figure 3-9: ME Debug Mode Jumper Location 29
Figure 3-10: iTPM Jumper Location 30
Figure 3-11: ME RTC Jumper Location 31
Figure 3-12: SPI Jumper Location 32
Figure 3-13: Wall-mounting Bracket 33
Figure 3-14: Chassis Support Screws 34
Figure 3-15: Securing the Panel PC 35
Figure 3-16: Arm Mounting Retention Screw Holes 36
Figure 3-17: LAN Connection 37
Figure 3-18: Serial Device Connector 38
Figure 3-19: USB Device Connection 39
Figure 3-20: VGA Connector 40
Figure 3-21: AT/ATX Switch Location 40
Figure4-1: HDD Bracket Screws 45
Figure 4-2: SO-DIMM Socket Location 45

Figure 4-3: DDR SO-DIMM Module Installation....46
Figure 4-4: HDD Cover Screw....47
Figure 4-5: HDD Bracket Retention Screw....47
Figure 4-6: HDD Removal....48
Figure 6-1: Chipset Driver File Extraction Screen....77
Figure 6-2: Chipset Driver Welcome Screen....77
Figure 6-3: Chipset Driver License Agreement....78
Figure 6-4: Readme File Information Screen....79
Figure 6-5: Setup Progress Screen....79
Figure 6-6: Chipset Driver Installation Finish Screen....80
Figure 6-7: VGA Driver Readme File....81
Figure 6-8: VGA Driver Setup File Extraction Screen....81
Figure 6-9: VGA Driver Welcome Screen....82
Figure 6-10: VGA Driver License Agreement....82
Figure 6-11: VGA Driver Readme File....83
Figure 6-12: VGA Driver Setup Operations....83
Figure 6-13: VGA Driver Setup Is Complete Screen....84
Figure 6-14: LAN Driver Welcome Screen....85
Figure 6-15: LAN Driver Welcome Screen....85
Figure 6-16: LAN Driver Installation....86
Figure 6-17: LAN Driver Installation Complete....86
Figure 6-18: The InstallShield Wizard Starts....87
Figure 6-19: Preparing Setup Screen....88
Figure 6-20: InstallShield Wizard Welcome Screen....88
Figure 6-21: Audio Driver Progress Screen....89
Figure 6-22: Installation Wizard Updates the System....89
Figure 6-23: Restart the Computer....90
Figure 6-24: PenMount Welcome Screen....91
Figure 6-25: License Agreement....91
Figure 6-26: Choose Install Location....92
Figure 6-27: Installing PenMount Universal Driver V2.1.0.263....92
Figure 6-28: PenMount Universal Driver Update Complete....93
Figure 6-29: Wireless Driver License Agreement....94
Figure 6-30: Wireless Driver Configuration Tool Options....94
Figure 6-31: Wireless Mode Select Window....95

Figure 6-32: Wireless Driver Installation 96
Figure 6-33: Keypad Driver Welcome Screen 97
Figure 6-34: Customer Information Screen 97
Figure 6-35: Setup Type 98
Figure 6-36: Ready to Install the Program 98
Figure 6-37: Installing KeypadAP v2.2 99
Figure 6-38: Keypad Driver Installation Complete Screen 99
Figure 6-39: Reboot the Computer 100

List of Tables

Table 1-1: System Specifications....8
Table 3-1: Jumpers....20
Table 3-2: Preconfigured Jumpers....21
Table 3-3: Clear CMOS Jumper Settings....21
Table 3-4: COM1 Pin 9 Setting Jumper Settings....22
Table 3-5: COM3 Pin 9 Setting Jumper Settings....23
Table 3-6: COM3 TX Function Select Jumper Settings....24
Table 3-7: COM3 RS-232/422/485 Serial Port Select Jumper Settings....26
Table 3-8: RS-422 Pinouts....27
Table 3-9: RS-485 Pinouts....27
Table 3-10: COM3 RX Function Select Jumper Settings....27
Table 3-11: ME Debug Mode Jumper Settings....28
Table 3-12: iTPM Jumper Settings....29
Table 3-13: ME RTC Jumper Settings....30
Table 3-14: SPI Jumper Settings....31
Table 5-1: BIOS Navigation Keys....51

BIOS Menus

BIOS Menu 1: Main 52
BIOS Menu 2: Advanced 54
BIOS Menu 3: ACPI Configuration 54
BIOS Menu 4: TPM Configuration 55
BIOS Menu 5: CPU Configuration 56
BIOS Menu 6: IDE Configuration 57
BIOS Menu 7: USB Configuration 58
BIOS Menu 8: Super IO Configuration 59
BIOS Menu 9: Serial Port n Configuration Menu 60
BIOS Menu 10: Hardware Health Configuration 64
BIOS Menu 11: Serial Port Console Redirection 65
BIOS Menu 12: Chipset 66
BIOS Menu 13: Northbridge Chipset Configuration 67
BIOS Menu 14: Southbridge Chipset Configuration 68
BIOS Menu 15: Intel IGD SWSCI OpRegion 69
BIOS Menu 16: Boot 71
BIOS Menu 17: Security 72
BIOS Menu 18: Exit 73

Chapter

1

Introduction

1.1 Overview

Figure 1-1: POC-17i/19i Series Medical Panel PC

The POC-17i/19i Series is an Intel® Core™ powered flat panel PC with a rich variety of functions and peripherals. All POC-17i/19i Series models are designed for easy and simplified integration into point-of-care (POC) applications.

An Intel® Core™ i7/i5/i3 processor coupled with the Intel® HM55 chipset delivers optimal memory, graphics, and peripheral I/O support. The system comes with 2.0 GB of preinstalled DDR3 dual-channel SO-DIMMs and supports a maximum of 8.0 GB ensuring smooth data throughputs with reduced bottlenecks and fast system access. The POC-17i/19i Series features a Gen 5.7 Enhanced Graphics Engine with 12 execution units and DirectX 10 and Open GL 2.1 support for high quality video performance. Dual display support is provided via VGA and HDMI ports.

Two serial ports and four external USB 2.0 ports provide simplified connectivity to a variety of external peripheral devices. Wi-Fi capabilities and two RJ-45 GbE connectors allow for smooth connection of the system to an external LAN. The POC-17i/19i Series also supports a 2.5” SATA HDD drive which can be accessed without removing the entire back panel.

Intended use: The POC-17i/19i Series is intended to serve as a medical computing device for integration with hospital system. It is designed for general purpose for hospital environment. For data collection and display for reference. It shall not be used for life-supporting system.

1.2 Features

The POC-17i/19i Series features the following:

- Intel® Core™ i7/i5/i3 processor
- Intel® HM55 chipset
- 2.0 GB DDR3 SO-DIMM preinstalled
- 802.11 a/b/g/n wireless module
- Four USB 2.0 ports
- Watchdog timer that triggers a system reset if the system hangs for some reason
- AT or ATX power mode
- Touch screen
- RoHS compliance

1.3 External Overview

1.3.1 General Description

The stylish POC-17i/19i Series panel PC is comprised of a screen, rear panel and bottom panel. An anti-bacteria plastic front frame surrounds the front screen. The rear panel provides screw holes for a wall-mounting bracket compliant with VESA FDMI standard. An I/O interface on the bottom panel provides access to external interface connectors that include LAN, USB 2.0, serial port, reset button, VGA, HDMI, audio connector, power connector, power switch and AT/ATX mode switch. The right side panel provides access to a SATA HDD drive.

1.3.2 Front Panel

The front side of the POC-17i/19i Series is a flat panel TFT LCD screen surrounded by an anti-bacteria plastic frame. The power LED is located at the top center of the front panel (**Figure 1-2**).

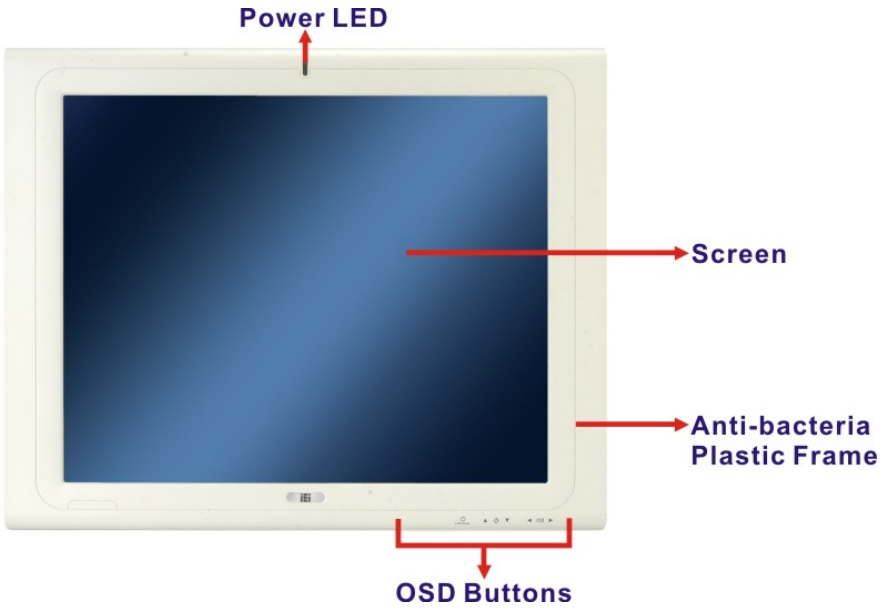

Figure 1-2: Front View

1.3.3 Rear Panel

The rear panel provides access to retention screw holes that support the wall mounting. Refer to **Figure 1-3**.

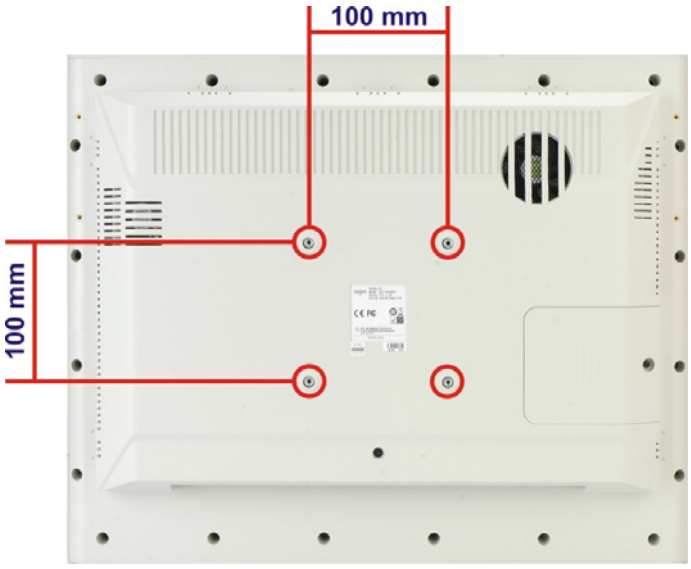

Figure 1-3: Rear View

1.3.4 I/O Interface Panel

The I/O interface panel located on the bottom of the POC-17i/19i Series has the following I/O interface connectors:

- 1 x Power switch
- 1 x 12 V DC In connector
- 1 x RS-232 connector
- 1 x RS-232/422/485 connector
- 2 x RJ-45 for Giga LAN connectors
- 1 x AT/ATX power mode switch
- 4 x USB 2.0 connectors
- 1 x HDMI connector
- 1 x Audio line-out connector
- 1 x VGA connector
- 1 x Reset button

The external I/O interface connector panel is shown in **Figure 1-4**.

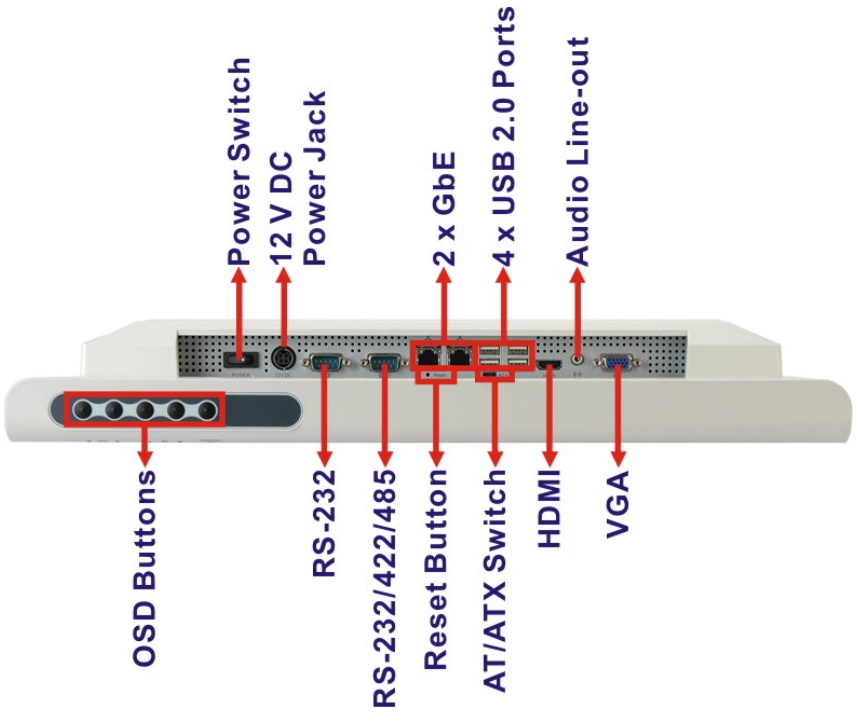

Figure 1-4: I/O Interface Connector Panel

1.3.5 OSD Control Buttons

The POC-17i/19i Series has seven OSD control buttons as shown below.

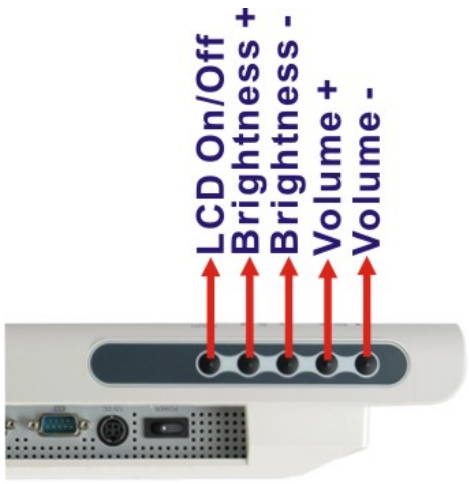

Figure 1-5: OSD Control Buttons

1.4 Internal Overview

The POC-17i/19i Series has the following components installed internally:

- 1 x Mainboard
- 1 x 2.0 GB 800/1066 MHz DDR3 SO-DIMM
- 1 x Wireless module
- 1 x 320GB SATA HDD

1.5 System Specifications

The technical specifications for the POC-17i/19i Series systems are listed in **Table 1-1.**

Specification	POC-17i	POC-19i
LCD Size	17”	19”
Max. Resolution	1280 x 1024	1280 x 1024
Brightness (cd/m^2)	350	350
LCD Color	16.7 M	16.7 M
Viewing Angle (H-V)	170 ◦ / 160 ◦	170 ◦ / 160 ◦
CPU	Intel® Celeron® P4500 1.86G CPU Intel® Core™ i3-330M 2.26G CPU Intel® Core™ i5-520M 2.4G CPU Intel® Core™ i7-620M 2.66G CPU	
Chipset	Intel® HM55	
Memory	One 204-pin 2 GB DDR3 SO-DIMM preinstalled (system max. 8GB, dual SO-DIMM slot)	
Speaker	AMP 3 W + AMP 3 W (built-in stereo speakers)	
Watchdog Timer	Software programmable supports 1 sec. ~ 255 sec. system reset	
Expansion	1 x PCIe Mini card (wireless LAN 802.11 a/b/g/n module)	
HDD Drive Bay	One 2.5” 320GB SATA HDD preinstalled	
Construction Material	Anti-bacteria plastic front frame	
Mounting	VESA 100 mm x 100 mm: Wall mounting Arm mounting	
Dimensions (mm) (W x H x D)	428 x 350 x 76	470 x 383 x 79
Operational Temperature	0ºC ~ 50ºC	
Storage/Transportation Temperature	-20ºC ~ 60ºC	
Operational Humidity	5% ~ 95%, non-condensing	
Storage/Transportation Humidity	5% ~ 95%, non-condensing	
Operational Pressure	700 hPa ~ 1060 hPa	
Storage/Transportation Pressure	500 hPa ~ 1060 hPa	
Net Weight	6.0kg	6.2kg
EMC	CE, FCC Class B	

Specification	POC-17i	POC-19i
Safety	ANSI/AAMI ES60601-1 CAN/CSA C22.2 No. 60601-1 IEC/EN 60601-1 3rd edition	
Touch Screen	Resistive Type 5-wire (touch controller is on board)	
Power Adapter (Medical Grade)	Manufacturer: FSP Group Inc.	
	Model: PMP120-12-S	
	Input: 100 V ~ 240 V, 47 Hz ~ 63 Hz, 1.4 A ~ 0.6 A	
	Output: 12 V, 8 A, 96 W	
System Rating	12 V, 8 A	
I/O Ports and Switches	1 x 12 V DC input jack	
	1 x Audio line-out connector	
	1 x RS-232 COM port connector	
	1 x RS-232/422/485 COM port connector	
	2 x RJ-45 for GbE LAN	
	1 x HDMI port	
	4 x USB 2.0 ports	
	1 x VGA connector	
	1 x Power switch	
	1 x Reset button	

Table 1-1: System Specifications

1.6 Dimensions

The POC-17i Series dimensions are shown in **Figure 1-6** and listed below.

- **Width**: 428 mm
- **Height**: 250.1 mm
- **Depth**: 76 mm (approximate)

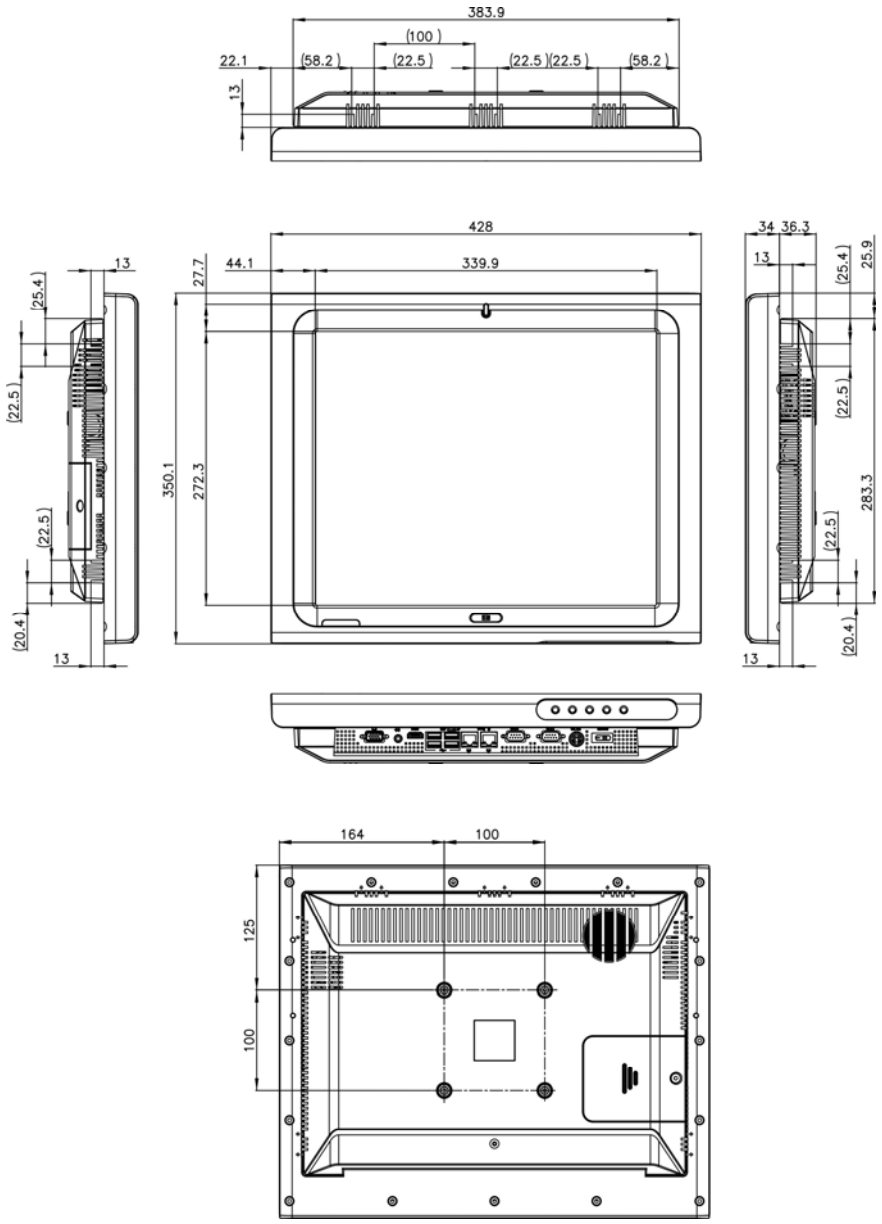

Figure 1-6: POC-17i Series Dimensions (mm)

The POC-19i Series dimensions are shown in **Figure 1-7** and listed below.

- **Width**: 469.9 mm
- **Height**: 382.5 mm
- **Depth**: 79 mm (approximate)

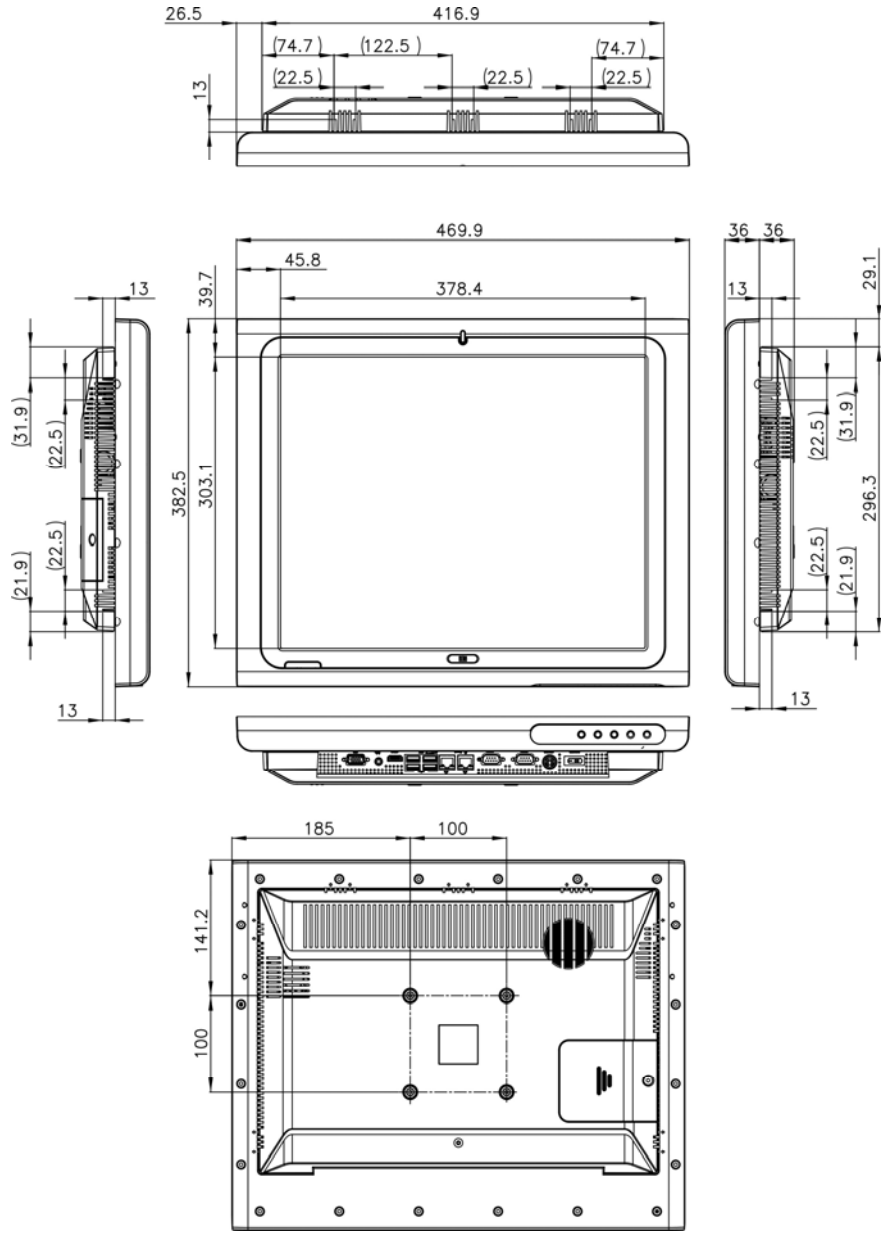

Figure 1-7: POC-17i Series Dimensions (mm)

Chapter

2

Unpacking

WARNING:

The labels on the external box are best to be read at a distance of 30 cm due to the small label size.

2.1 Unpacking

To unpack the flat panel PC, follow the steps below:

WARNING!

The front side LCD screen has a protective plastic cover stuck to the screen. Only remove the plastic cover after the flat panel PC has been properly installed. This ensures the screen is protected during the installation process.

Step 1: Use box cutters, a knife or a sharp pair of scissors that seals the top side of the external (second) box.

Step 2: Open the external (second) box.

Step 3: Use box cutters, a knife or a sharp pair of scissors that seals the top side of the internal (first) box.

Step 4: Lift the monitor out of the boxes.

Step 5: Remove both polystyrene ends, one from each side.

Step 6: Pull the plastic cover off the flat panel PC.

Step 7: Make sure all the components listed in the packing list are present.

2.2 Packing List

The POC-17i/19i Series flat panel PC is shipped with the following components:

NOTE:

If any of these items are missing or damaged, contact the distributor or sales representative immediately.

Quantity	Item	Image
Standard		
1	POC-17i/19i Series	
1	Medical-grade power adapter	
1	Power cord	
1	Screw kit	

1	Touch pen	
1	User manual CD and driver CD	

Chapter

3

Installation

3.1 Anti-static Precautions

WARNING:

Failure to take ESD precautions during the maintenance of the device may result in permanent damage to the device and severe injury to the user.

Electrostatic discharge (ESD) can cause serious damage to electronic components, including the POC-17i/19i Series. Dry climates are especially susceptible to ESD. It is therefore critical that whenever the POC-17i/19i Series is accessed internally, or any other electrical component is handled, the following anti-static precautions are strictly adhered to.

- ***Wear an anti-static wristband***: - Wearing a simple anti-static wristband can help to prevent ESD from damaging the board.
- ***Self-grounding***: - Before handling the board touch any grounded conducting material. During the time the board is handled, frequently touch any conducting materials that are connected to the ground.
- ***Use an anti-static pad***: - When configuring the POC-17i/19i Series, place it on an antic-static pad. This reduces the possibility of ESD damaging the device.
- ***Only handle the edges of the PCB***: - When handling the PCB, hold the PCB by the edges.

3.2 Installation Precautions

When installing the flat panel PC, please follow the precautions listed below:

- **Power turned off**: When installing the flat panel PC, make sure the power is off. Failing to turn off the power may cause severe injury to the body and/or damage to the system.
- **Certified Engineers**: Modification to the product is not permitted unless with authorization of the company, certified engineer does not mean he/she has the authority from the company, so remove the modification part.

- **Anti-static Discharge**: If a user open the rear panel of the flat panel PC, to configure the jumpers or plug in added peripheral devices, ground themselves first and wear and anti-static wristband.

3.3 Installation and Configuration Steps

The following installation steps must be followed.

Step 1: Remove the rear panel cover

Step 2: Remove the internal aluminum cover

Step 3: Configure the system jumpers

Step 4: Connect peripheral devices to the bottom panel of the flat panel PC

Step 5: Mount the flat panel PC

3.4 Removing the Rear Panel Cover

WARNING:

Over-tightening rear cover screws will crack the plastic frame. Maximum torque for cover screws is 5 kg-cm (0.36 lb-ft/0.49 Nm).

To access the POC-17i/19i Series internally, the rear panel cover must first be removed. To remove the rear panel cover, please follow the steps below.

Step 1: Remove twenty-one (21) retention screws from the rear panel cover. See **Figure 3-1**.

Figure 3-1: Back Cover Retention Screws

Step 2: Lift the cover off the POC-17i/19i Series panel PC.

3.5 Removing the Internal Aluminum Cover

WARNING:

Over-tightening rear cover screws will crack the plastic frame. Maximum torque for cover screws is 5 kg-cm (0.36 lb-ft/0.49 Nm).

To remove the internal aluminum cover, follow the steps below.

Step 1: Remove retention screws securing the internal aluminum cover.

Step 2: **Figure 3-2** shows the aluminum cover retention screws of the POC-17i/19i Series.

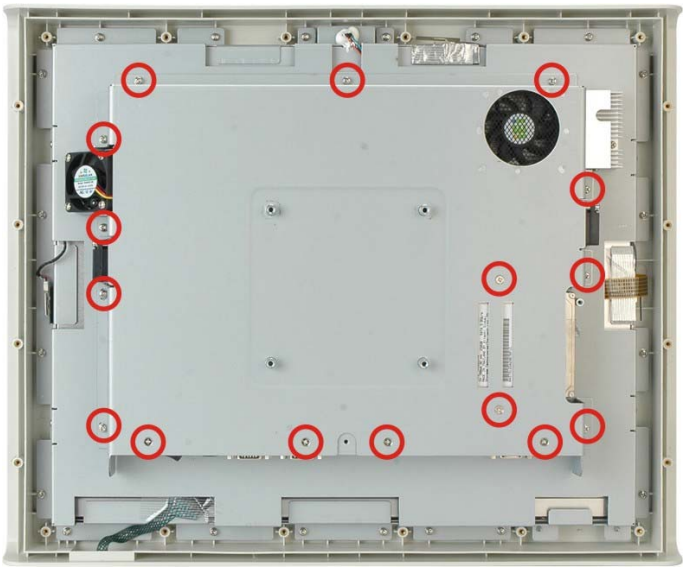

Figure 3-2: Aluminum Back Cover Retention Screws

Step 3: Lift the aluminum cover away to expose the mainboard jumpers.

3.6 Jumper Settings

NOTE:

A jumper is a metal bridge used to close an electrical circuit. It consists of two or three metal pins and a small metal clip (often protected by a plastic cover) that slides over the pins to connect them. To CLOSE/SHORT a jumper means connecting the pins of the jumper with the plastic clip and to OPEN a jumper means removing the plastic clip from a jumper.

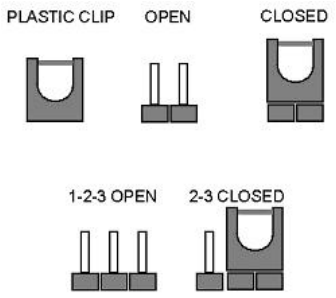

The following jumpers can be found on the motherboard installed in the POC-17i/19i Series. Before the POC-17i/19i Series is installed, the jumpers must be set in accordance with the desired configuration. The jumpers on the POC-17i/19i Series motherboard are listed in **Table 3-1**.

Description	Label	Type
Clear CMOS setting	J_CMOS1	3-pin header
COM1 Pin 9 setting	JP7, JP8	6-pin header
COM3 TX function select	JP9	6-pin header
COM3 RS-232/422/485	JP10	12-pin header
COM3 RS function select	JP11	8-pin header
ME Debug Mode	JP12	2-pin header
iTPM setting	J_ITPM1	3-pin header
ME RTC select	ME_RTC1	3-pin header
SPI setting	J_SPI1	3-pin header

Table 3-1: Jumpers

3.6.1 Access the Jumpers

To access the jumpers, please remove the back panel and the internal aluminum chassis (see **Section 3.4** and **Section 3.5**).

3.6.2 Preconfigured Jumpers

WARNING:

Do not change the settings on the jumpers in described here. Doing so may disable or damage the system.

The following jumpers are preconfigured for the POC-17i/19i Series. Users should not change these jumpers (**Table 3-2**).

Jumper Name	Label	Type
MCU Detect LCD Type	JP3	4-pin header

MCU PWM Power	JP4	3-pin header
LCD Power Select	J_VLVDS1	6-pin header

Table 3-2: Preconfigured Jumpers

3.6.3 Clear CMOS Jumper

Jumper Label: **J_CMOS1**

Jumper Type: 3-pin header

Jumper Settings: See **Table 3-3**

Jumper Location: See **Figure 3-3**

If the POC-17i/19i Series fails to boot due to improper BIOS settings, the clear CMOS jumper clears the CMOS data and resets the system BIOS information. To do this, use the jumper cap to close the pins for a few seconds then remove the jumper clip.

If the "CMOS Settings Wrong" message is displayed during the boot up process, the fault may be corrected by pressing F1 to enter the CMOS Setup menu. Do one of the following:

- Enter the correct CMOS setting
- Load Optimal Defaults
- Load Failsafe Defaults.

After having done one of the above, save the changes and exit the CMOS Setup menu.

The clear CMOS jumper settings are shown in **Table 3-3**.

Clear CMOS	Description
Short 1 - 2	Keep CMOS Setup
Short 2 - 3	Clear CMOS Setup

Table 3-3: Clear CMOS Jumper Settings

The location of the clear CMOS jumper is shown in **Figure 3-3** below.

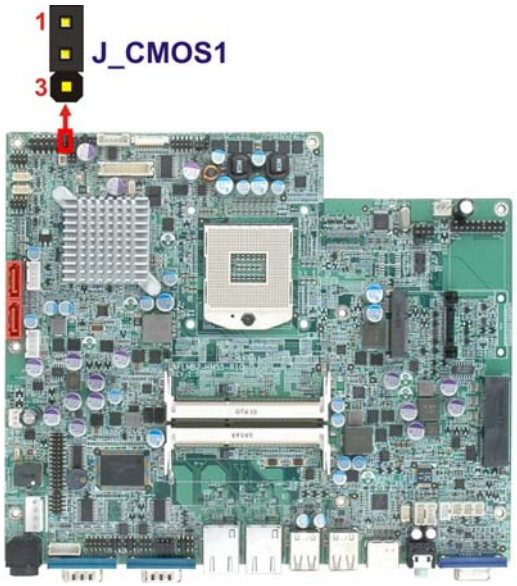

Figure 3-3: Clear CMOS Jumper

3.6.4 COM1 Pin 9 Setting

Jumper Label:	**JP7 and JP8**
Jumper Type:	6-pin header
Jumper Settings:	See **Table 3-4** and **Table 3-5**
Jumper Location:	See **Figure 3-4** and **Figure 3-5**

Two jumpers (JP7 and JP8) configure pin 9 on COM1 and COM3 DB-9 connectors. Pin 9 on the COM1 and the COM3 DB-9 connectors can be set as the ring (RI) signal, +5 V or +12 V. The COM1 and COM3 Pin 9 Setting jumper selection options are shown in the tables below.

JP7	Description
Short 1-2	COM1 RI +12 V
Short 3-4	COM1 RI Normal
Short 5-6	COM1 RI Pin +5 V

Table 3-4: COM1 Pin 9 Setting Jumper Settings

The JP7 jumper location is shown below.

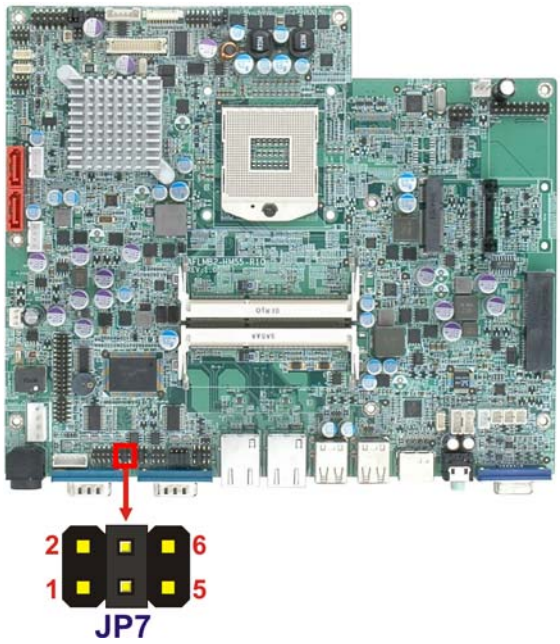

Figure 3-4: JP7 Jumper Setting Location

JP8	Description
Short 1-2	COM3 RI +12 V
Short 3-4	COM3 RI Normal
Short 5-6	COM3 RI +5 V

Table 3-5: COM3 Pin 9 Setting Jumper Settings

The JP8 jumper location is shown below.

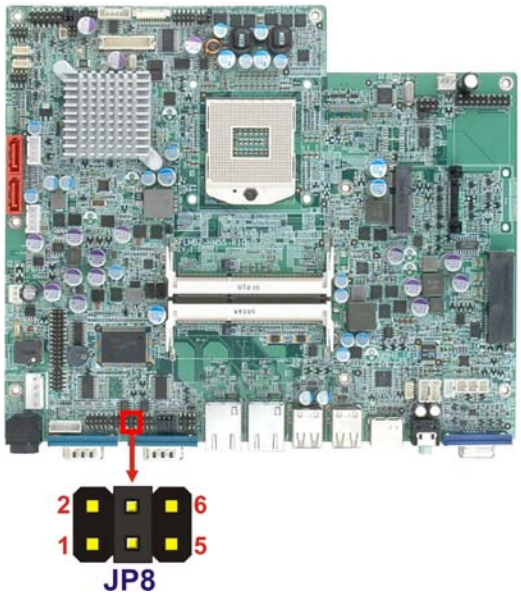

Figure 3-5: JP8 Jumper Setting Location

3.6.5 COM3 TX Function Select Jumper

Jumper Label: **JP9**

Jumper Type: 6-pin header

Jumper Settings: See **Table 3-6**

Jumper Location: See **Figure 3-6**

The COM3 TX Function Select jumper configures the TX pin on COM3 serial port connector as RS-422 or RS-485. The COM3 TX Function Select jumper selection options are shown in **Table 3-6**.

JP9	Description
Short 1 – 3	RS-422 TX-
Short 2 – 4	RS-422 TX+
Short 3 – 5	RS-485 D-
Short 4 – 6	RS-485 D+

Table 3-6: COM3 TX Function Select Jumper Settings

The COM3 TX Function Select jumper location is shown in **Figure 3-6** below.

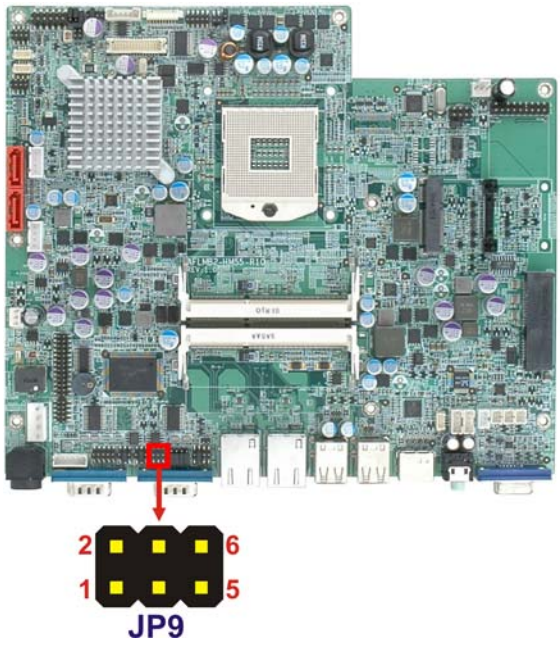

Figure 3-6: COM3 TX Function Select Jumper Location

3.6.6 COM3 RS-232/422/485 Jumper

Jumper Label:	**JP10**
Jumper Type:	12-pin header (four 3-pin headers combined)
Jumper Settings:	See **Table 3-7**
Jumper Location:	See **Figure 3-7**

The COM3 RS-232/422/485 Serial Port Select jumper sets the communication protocol used by the second serial communications port (COM3) as RS-232, RS-422 or RS-485. The COM3 RS-232/422/485 Serial Port Select settings are shown in **Table 3-7**.

JP10	Description
Short 1-2	RS-232
Short 4-5	RS-232
Short 7-8	RS-232

Short 10-11	RS-232
Short 2-3	RS-422/485
Short 5-6	RS-422/485
Short 8-9	RS-422/485
Short 11-12	RS-422/485

Table 3-7: COM3 RS-232/422/485 Serial Port Select Jumper Settings

The COM3 RS-232/422/485 Serial Port Select jumper location is shown in **Figure 3-7**.

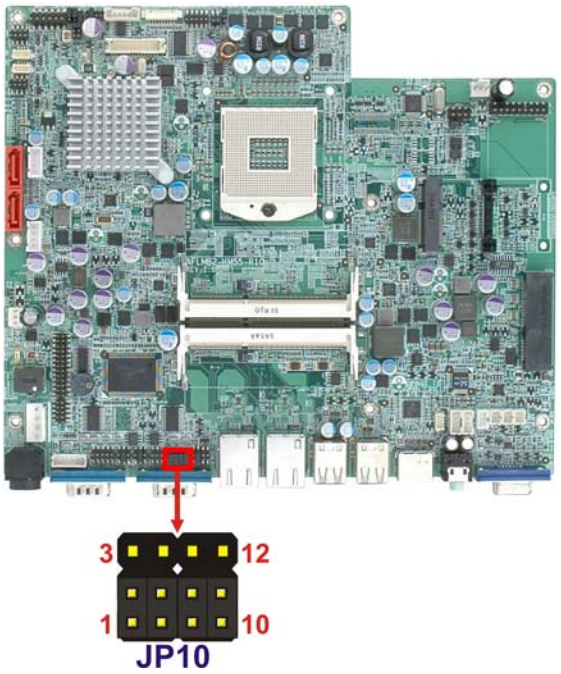

Figure 3-7: COM3 RS-232/422/485 Serial Port Select Jumper Location

3.6.6.1 COM3 RS-422 and RS-485 Pinouts

The pinouts for RS-422 and RS-485 operation of external serial port COM 3 are detailed below.

COM 3	RS-422 Description
Pin 1	TX-
Pin 2	TX+
Pin 6	RX-

Pin 7	RX+

Table 3-8: RS-422 Pinouts

COM 3	RS-485 Description
Pin 1	Data-
Pin 2	Data+

Table 3-9: RS-485 Pinouts

3.6.7 COM3 RS Function Select Jumper

Jumper Label: **JP11**

Jumper Type: 8-pin header

Jumper Settings: See **Table 3-10**

Jumper Location: See **Figure 3-8**

The COM3 RX Function Select jumper sets the communication protocol used by the RX serial communications port COM3 as RS-232, RS-422 or RS-485. The COM3 RX Function Select jumper settings are shown in **Table 3-10**.

COM3 RX Function Select	Description
Short 1-2	DET BIOS RS232/422/485
Short 3-4	RS-232
Short 5-6	RS-422
Short 7-8	RS-485

Table 3-10: COM3 RX Function Select Jumper Settings

The COM3 RX Function Select jumper location is shown in **Figure 3-8**.

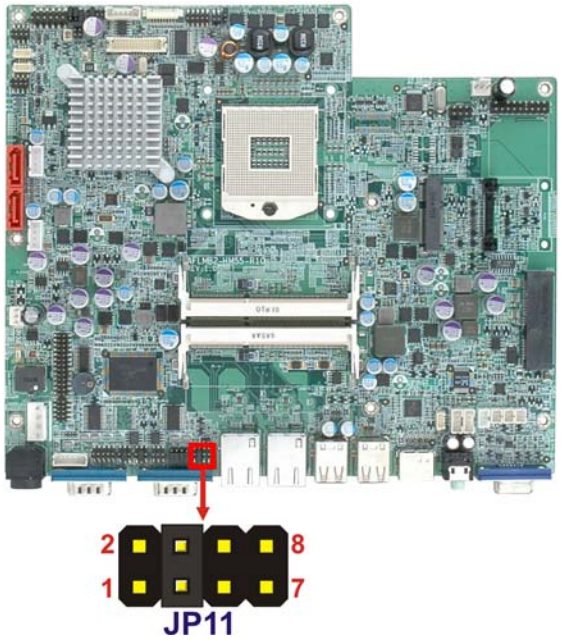

Figure 3-8: COM3 RX Function Select Jumper Location

3.6.8 ME Debug Mode Jumper

Jumper Label:	**JP12**
Jumper Type:	2-pin header
Jumper Settings:	See **Table 3-11**
Jumper Location:	See **Figure 3-9**

The ME Debug Mode jumper allows ME firmware overwrite protection. The ME Debug Mode jumper settings are shown in **Table 3-11**.

ME Debug Mode	Description
Open	Disabled
Closed	Enabled

Table 3-11: ME Debug Mode Jumper Settings

The ME Debug Mode jumper location is shown in **Figure 3-9**.

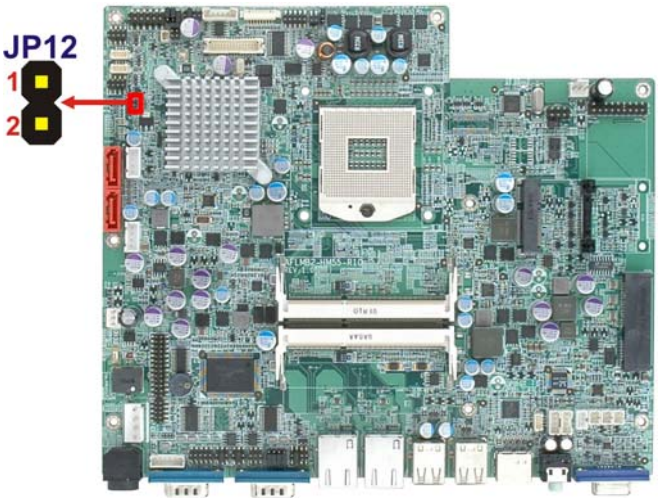

Figure 3-9: ME Debug Mode Jumper Location

3.6.9 iTPM Setting Jumper

Jumper Label:	**J_ITPM1**
Jumper Type:	3-pin header
Jumper Settings:	See **Table 3-12**
Jumper Location:	See **Figure 3-10**

The iTPM jumper settings are shown in **Table 3-12**.

iTPM setting	Description
Short 1-2	Disable iTPM
Short 2-3	Enable iTPM

Table 3-12: iTPM Jumper Settings

The iTPM jumper location is shown in **Figure 3-10**.

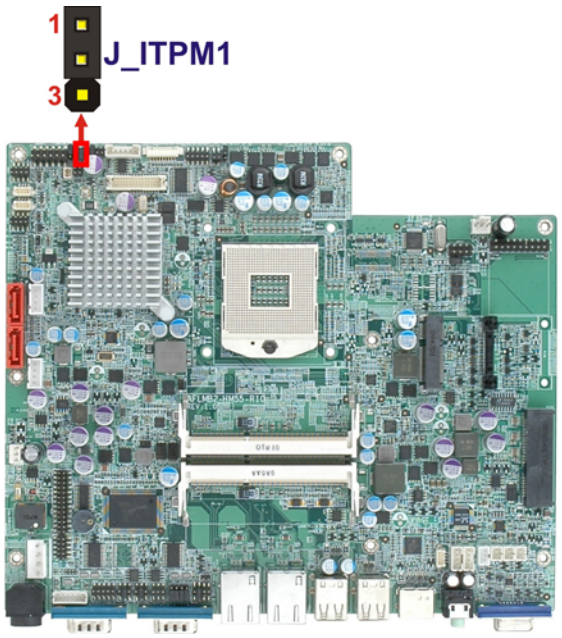

Figure 3-10: iTPM Jumper Location

3.6.10 ME RTC Select Jumper

Jumper Label:	**ME_RTC1**
Jumper Type:	3-pin header
Jumper Settings:	See **Table 3-13**
Jumper Location:	See **Figure 3-11**

The ME RTC select jumper settings are shown in **Table 3-13**.

ME RTC select	Description
Short 1-2	Keep ME RTC
Short 2-3	Clear ME RTC

Table 3-13: ME RTC Jumper Settings

The ME RTC jumper location is shown in **Figure 3-11**.

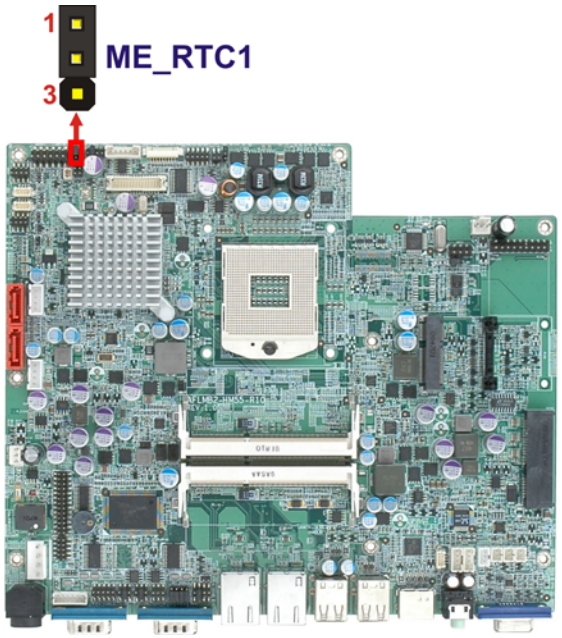

Figure 3-11: ME RTC Jumper Location

3.6.11 SPI Setting Jumper

Jumper Label:	**J_SPI**
Jumper Type:	3-pin header
Jumper Settings:	See **Table 3-14**
Jumper Location:	See **Figure 3-12**

The SPI jumper settings are shown in **Table 3-14**.

SPI setting	Description
Short 1-2	Program SP10
Short 2-3	Program SPI1

Table 3-14: SPI Jumper Settings

The SPI jumper location is shown in **Figure 3-12**.

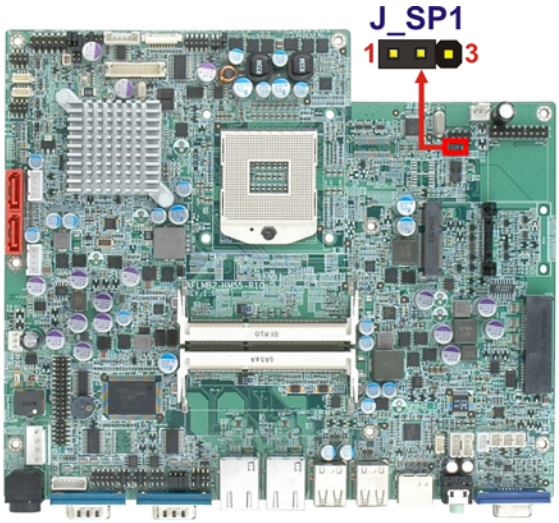

Figure 3-12: SPI Jumper Location

3.7 Mounting the System

WARNING!

When mounting the flat panel PC onto an arm, onto the wall or onto a panel, it is better to have more than one person to help with the installation to make sure the panel PC does not fall down and get damaged.

The methods of mounting the POC-17i/19i Series are listed below.

- Wall mounting
- Arm mounting

The mounting methods are described below.

3.7.1 Wall Mounting

To mount the flat panel PC onto the wall, please follow the steps below.

Step 1: Select the location on the wall for the wall-mounting bracket.

Step 2: Carefully mark the locations of the four screw holes in the bracket on the wall.

Step 3: Drill four pilot holes at the marked locations on the wall for the bracket retention screws.

Step 4: Align the wall-mounting bracket screw holes with the pilot holes.

Step 5: Secure the mounting-bracket to the wall by inserting the retention screws into the four pilot holes and tightening them (**Figure 3-13**).

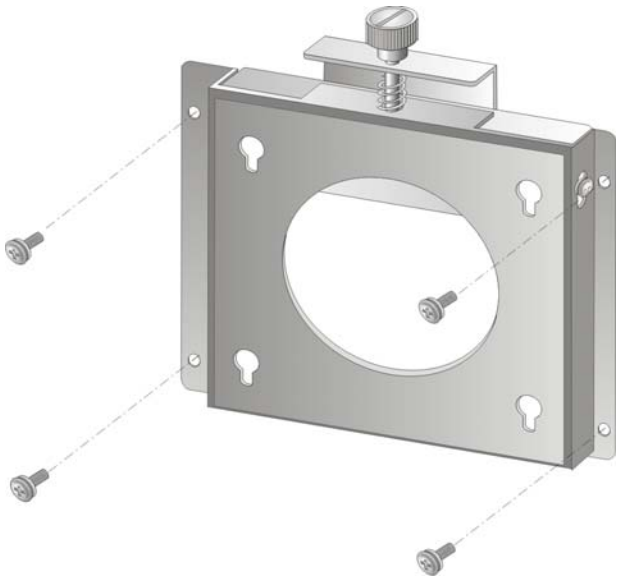

Figure 3-13: Wall-mounting Bracket

Step 6: Insert the four monitor mounting screws provided in the wall mounting kit into the four screw holes on the real panel of the flat panel PC and tighten until the screw shank is secured against the rear panel (**Figure 3-14**).

Step 7: Align the mounting screws on the monitor rear panel with the mounting holes on the bracket.

Step 8: Carefully insert the screws through the holes and gently pull the monitor downwards until the monitor rests securely in the slotted holes (**Figure 3-14**). Ensure that all four of the mounting screws fit snuggly into their respective slotted holes.

NOTE:

In the diagram below the bracket is already installed on the wall.

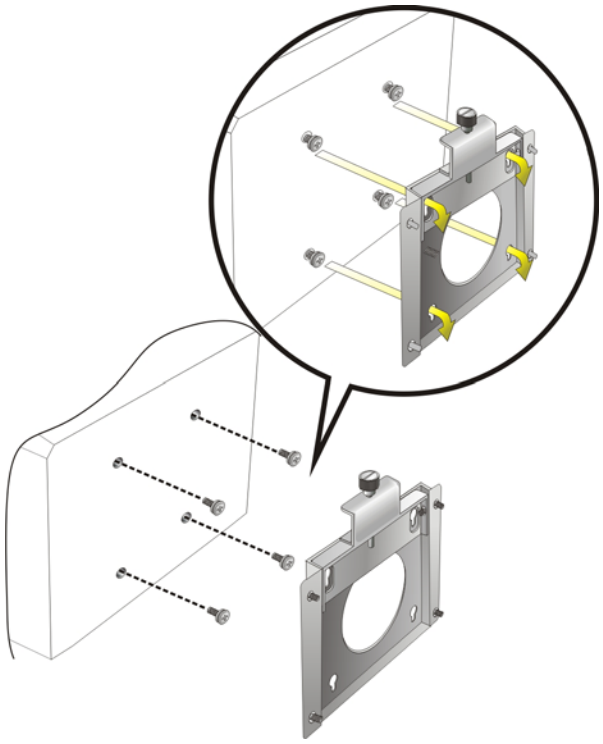

Figure 3-14: Chassis Support Screws

Step 9: Secure the panel PC by fastening the retention screw of the wall-mounting bracket. (**Figure 3-15**).

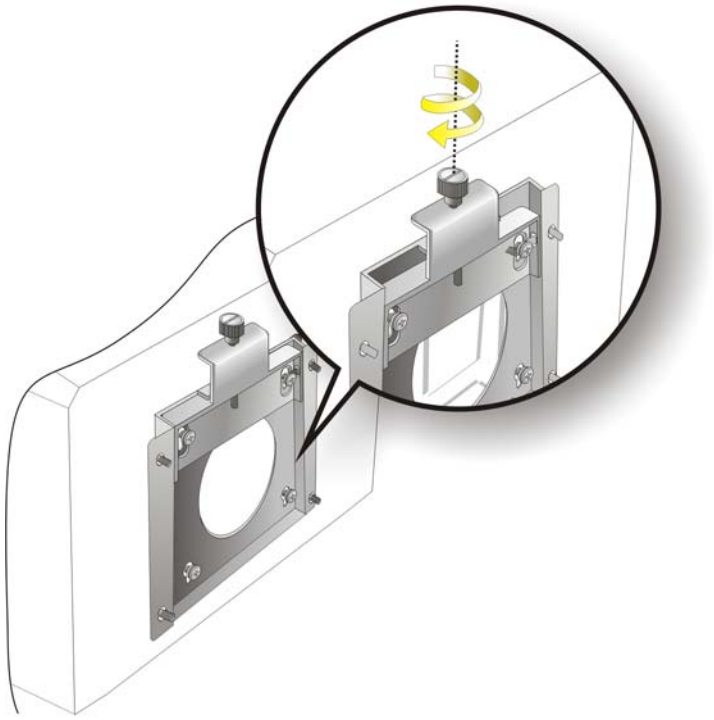

Figure 3-15: Securing the Panel PC

3.7.2 Arm Mounting

The POC-17i/19i Series is VESA (Video Electronics Standards Association) compliant and can be mounted on an arm with a 75mm or 100mm interface pad. To mount the POC-17i/19i Series on an arm, please follow the steps below.

Step 1: The arm is a separately purchased item. Please correctly mount the arm onto the surface it uses as a base. To do this, refer to the installation documentation that came with the mounting arm.

NOTE:

When purchasing the arm please ensure that it is VESA compliant and that the arm has a 100 mm interface pad. If the mounting arm is not VESA compliant it cannot be used to support the POC-17i/19i Series flat panel PC.

Step 2: Once the mounting arm has been firmly attached to the surface, lift the flat panel PC onto the interface pad of the mounting arm.

Step 3: Align the retention screw holes on the mounting arm interface with those in the flat panel PC. The POC-17i/19i Series arm mount retention screw holes are shown in **Figure 3-16**.

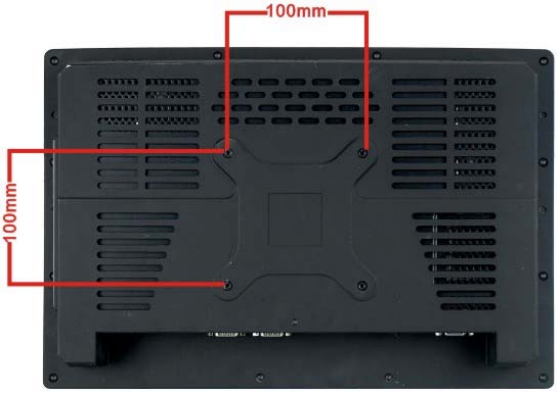

Figure 3-16: Arm Mounting Retention Screw Holes

Step 4: Secure the flat panel PC to the interface pad by inserting four retention screws through the bottom of the mounting arm interface pad and into the flat panel PC.

3.8 Bottom Panel Connectors

3.8.1 LAN Connection

There are two external RJ-45 LAN connectors. The RJ-45 connector enables connection to an external network. To connect a LAN cable with an RJ-45 connector, please follow the instructions below.

Step 1: **Locate the RJ-45 connectors** on the bottom panel of the POC-17i/19i Series.

Step 2: **Align the connectors.** Align the RJ-45 connector on the LAN cable with one of the RJ-45 connectors on the bottom panel of the POC-17i/19i Series. See **Figure 3-17**.

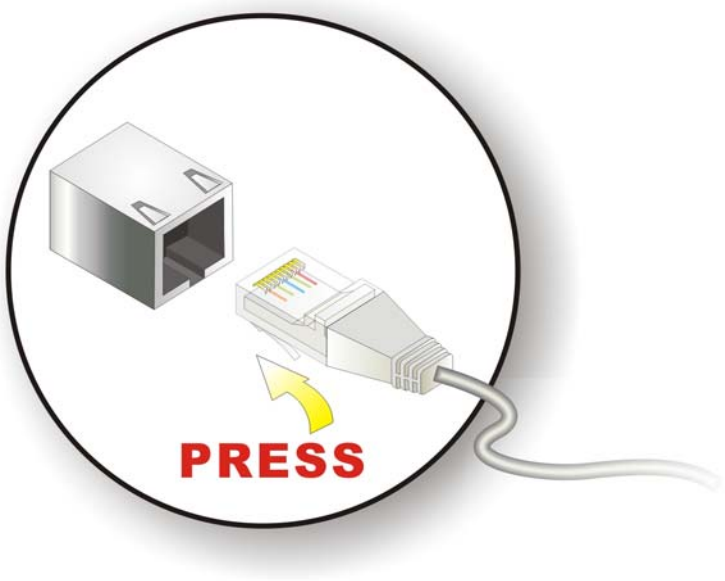

Figure 3-17: LAN Connection

Step 3: **Insert the LAN cable RJ-45 connector.** Once aligned, gently insert the LAN cable RJ-45 connector into the onboard RJ-45 connector.

3.8.2 Serial Device Connection

The POC-17i/19i Series has two male DB-9 connectors on the bottom panel for serial devices to be connected. Follow the steps below to connect a serial device to the POC-17i/19i Series panel PC.

Step 1: **Locate the DB-9 connector**. The location of the DB-9 connector is shown in **Chapter 2**.

Step 2: **Insert the serial connector**. Insert the DB-9 connector of a serial device into the DB-9 connector on the bottom panel. See **Figure 3-18**.

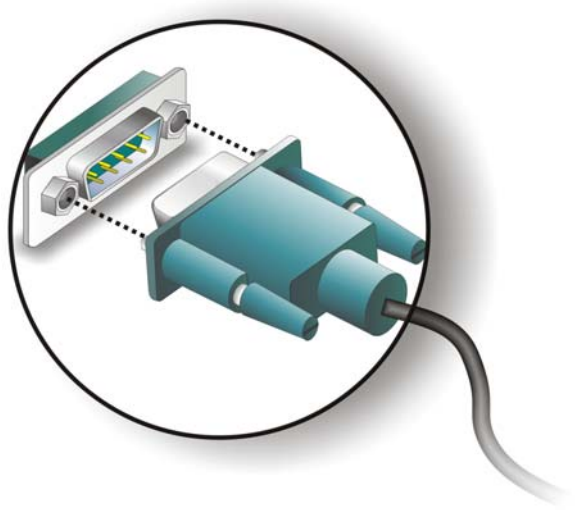

Figure 3-18: Serial Device Connector

Step 3: **Secure the connector**. Secure the serial device connector to the external interface by tightening the two retention screws on either side of the connector.

3.8.3 USB Device Connection

There are four external USB 2.0 connectors. All connectors are perpendicular to the POC-17i/19i Series. To connect a USB 2.0 or USB 1.1 device, please follow the instructions below.

Step 1: **Located the USB connectors**. The locations of the USB connectors are shown in **Chapter 2**.

Step 2: **Align the connectors.** Align the USB device connector with one of the connectors on the bottom panel. See **Figure 3-19**.

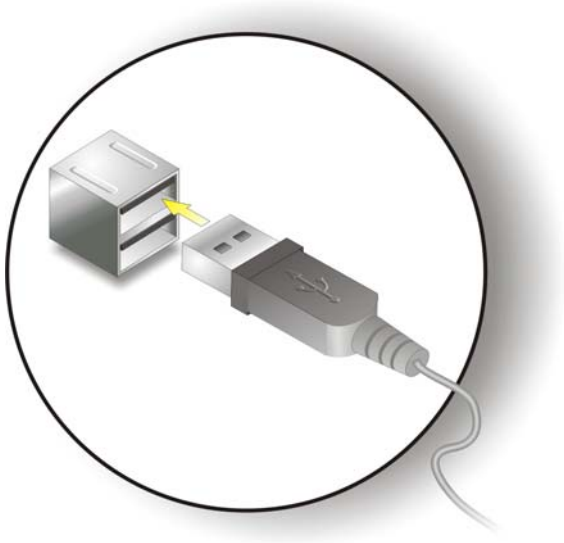

Figure 3-19: USB Device Connection

Step 3: **Insert the device connector.** Once aligned, gently insert the USB device connector into the onboard connector.

3.8.4 VGA Monitor Connection

The POC-17i/19i Series has a single female DB-15 connector on the external peripheral interface panel. The DB-15 connector is connected to a CRT or VGA monitor. To connect a monitor to the POC-17i/19i Series, please follow the instructions below.

Step 1: Locate the female DB-15 connector. The location of the female DB-15 connector is shown in Section 1.3.4.

Step 2: **Align the VGA connector**. Align the male DB-15 connector on the VGA screen cable with the female DB-15 connector on the external peripheral interface.

Step 3: **Insert the VGA connector** Once the connectors are properly aligned with the insert the male connector from the VGA screen into the female connector on the POC-17i/19i Series. See Figure 3-20.

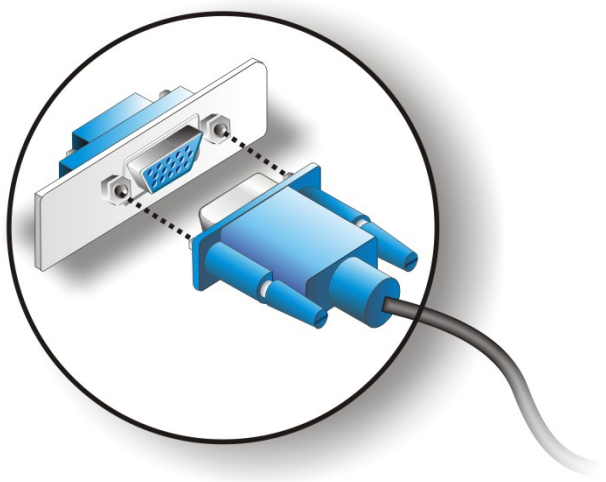

Figure 3-20: VGA Connector

Step 4: **Secure the connector**. Secure the DB-15 VGA connector from the VGA monitor to the external interface by tightening the two retention screws on either side of the connector.

3.9 AT/ATX Mode Selection

AT and ATX power modes can both be used on the POC-17i/19i Series. The selection is made through an AT/ATX switch on bottom panel (**Figure 3-21**). To select AT mode or ATX mode, follow the steps below.

Step 1: Locate the AT/ATX switch on the bottom panel (**Figure 3-21**).

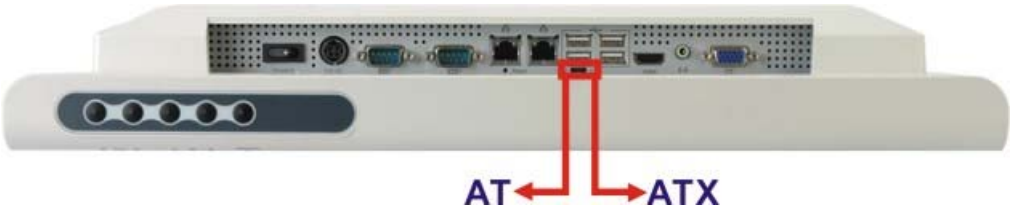

Figure 3-21: AT/ATX Switch Location

Step 2: Adjust the switch according to the preferred setting.

3.9.1 AT Power Mode

With the AT mode selected, the power is controlled by a central power unit rather than a power switch. The POC-17i/19i Series panel PC turns on automatically when the power is connected. The AT mode benefits a production line to control multiple panel PCs from a central management center and other applications including:

- ATM
- Self-service kiosk
- Plant environment monitoring system
- Factory automation platform
- Manufacturing shop flow

3.9.2 ATX Power Mode

With the ATX mode selected, the POC-17i/19i Series panel PC goes in a standby mode when it is turned off. The panel PC can be easily turned on via network or a power switch in standby mode. Remote power control is perfect for advertising applications since the broadcasting time for each panel PC can be set individually and controlled remotely. Other possible application includes

- Security surveillance
- Point-of-Sale (POS)
- Advertising terminal

Chapter

4

System Maintenance

4.1 System Maintenance Introduction

If the components of the POC-17i/19i Series fail they must be replaced. Components that can be replaced include:

- SO-DIMM module
- HDD drive

Please contact the system reseller or vendor to purchase replacement parts.

4.2 Anti-static Precautions

WARNING:

Failure to take ESD precautions during the maintenance of the POC-17i/19i Series may result in permanent damage to the POC-17i/19i Series and severe injury to the user.

Electrostatic discharge (ESD) can cause serious damage to electronic components, including the POC-17i/19i Series. Dry climates are especially susceptible to ESD. It is therefore critical that whenever the panel PC is accessed internally, or any other electrical component is handled, the following anti-static precautions are strictly adhered to.

- ***Wear an anti-static wristband***: - Wearing a simple anti-static wristband can help to prevent ESD from damaging the board.
- ***Self-grounding***: - Before handling the board touch any grounded conducting material. During the time the board is handled, frequently touch any conducting materials that are connected to the ground.
- ***Use an anti-static pad***: - When configuring the POC-17i/19i Series, place it on an antic-static pad. This reduces the possibility of ESD damaging the POC-17i/19i Series.
- ***Only handle the edges of the PCB***: - When handling the PCB, hold the PCB by the edges.

4.3 Turn off the Power

WARNING:

Failing to turn off the system before opening it can cause permanent damage to the system and serious or fatal injury to the user.

Before any maintenance procedures are carried out on the system, make sure the system is turned off.

4.4 Replacing Components

4.4.1 Memory Module Replacement

The flat panel PC features two DDR3 dual-channel SO-DIMM sockets supporting a system max of 8GB. If the memory module fails, follow the instructions below to replace the memory module.

Step 1: Remove the back cover. See **Section 3.4.**

Step 2: Remove the internal aluminum back cover. See **Section 3.5**.

Step 3: Remove four (4) retention screws securing the HDD bracket to the chassis. See the following figure.

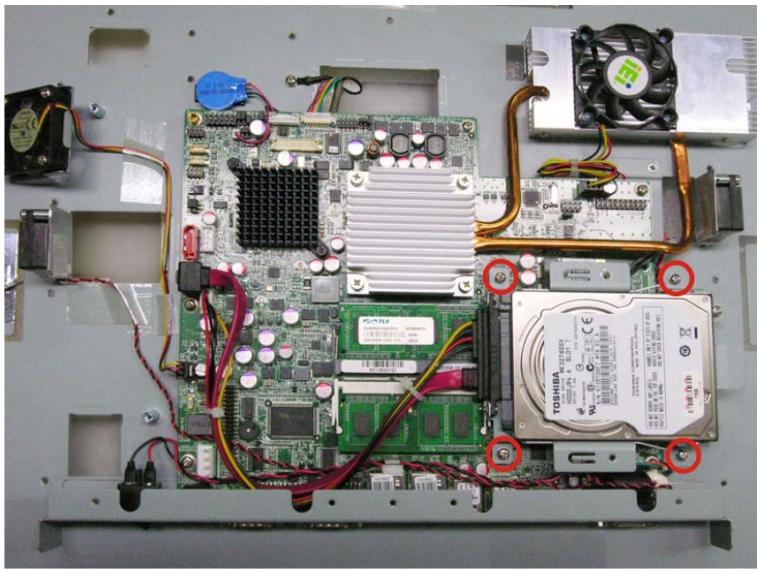

Figure 4-1: HDD Bracket Screws

Step 4: Lift the HDD bracket away to expose the DIMM connectors. See (**Figure 4-2**).

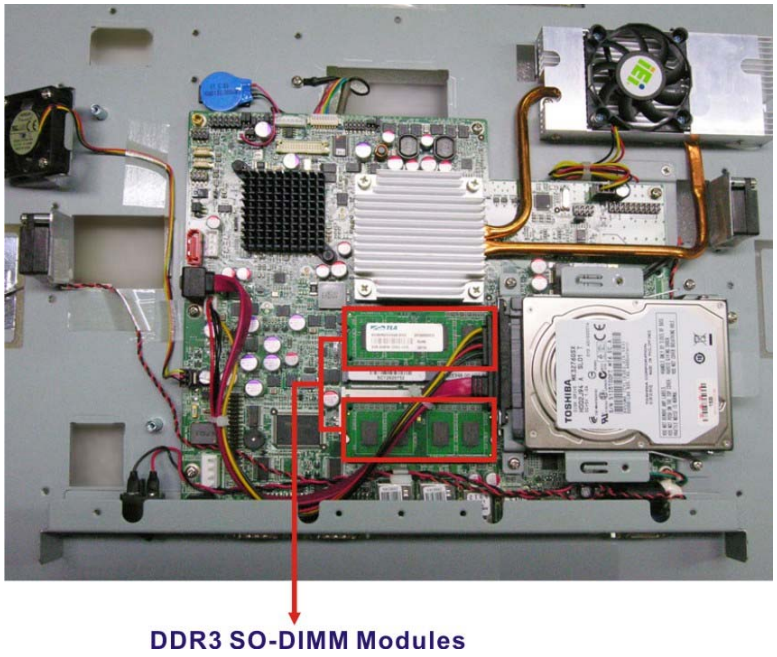

Figure 4-2: SO-DIMM Socket Location

Step 5: Remove the DDR memory module by pulling both the spring retainer clips outward from the socket.

Step 6: Grasp the DDR memory module by the edges and carefully pull it out of the socket.

Step 7: Install the new DDR memory module by pushing it into the socket at an angle (**Figure 4-3**).

Step 8: Gently pull the spring retainer clips of the SO-DIMM socket out and push the rear of the DDR memory module down (**Figure 4-3**).

Step 9: Release the spring retainer clips on the SO-DIMM socket. They clip into place and secure the DDR memory module in the socket.

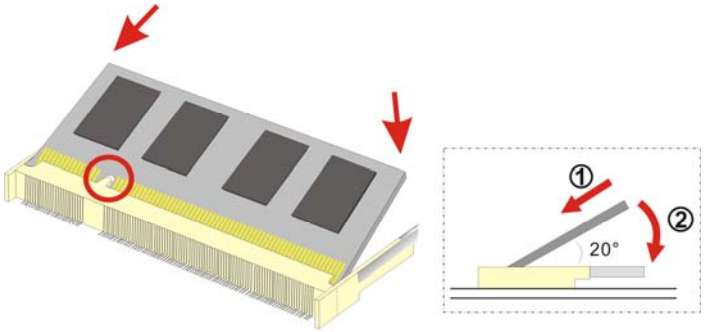

Figure 4-3: DDR SO-DIMM Module Installation

4.4.2 HDD Card Replacement

The POC-17i/19i Series is preinstalled with one HDD. To replace the HDD, follow the instructions below.

Step 1: Follow all anti-static procedures. See **Section 4.2**.

Step 2: Turn off the power. See **Section 4.3**.

Step 3: Remove the HDD cover by removing the HDD cover screw.

Figure 4-4: HDD Cover Screw

Step 4: Remove the HDD bracket retention screw (**Figure 4-4**).

Figure 4-5: HDD Bracket Retention Screw

Step 5: Pull the old HDD from the HDD slot.

Figure 4-6: HDD Removal

Step 6: Line up the new HDD with the SATA connector.

Step 7: Insert the HDD into SATA connector until it is securely in place.

Step 8: Secure the HDD bracket with the previously removed retention screw.

Step 9: Replace the HDD cover and secure using one (1) retention screw.

Chapter

5

BIOS Setup

5.1 Introduction

A licensed copy of the BIOS is preprogrammed into the ROM BIOS. The BIOS setup program allows users to modify the basic system configuration. This chapter describes how to access the BIOS setup program and the configuration options that may be changed.

5.1.1 Starting Setup

The UEFI BIOS is activated when the computer is turned on. The setup program can be activated in one of two ways.

1. Press the **DELETE** or **F2** key as soon as the system is turned on or
2. Press the **DELETE** or **F2** key when the "**Press Del to enter SETUP**" message appears on the screen.

If the message disappears before the **DELETE** or **F2** key is pressed, restart the computer and try again.

5.1.2 Using Setup

Use the arrow keys to highlight items, press **ENTER** to select, use the PageUp and PageDown keys to change entries, press **F1** for help and press **ESC** to quit. Navigation keys are shown in the following table.

Key	Function
Up arrow	Move to the item above
Down arrow	Move to the item below
Left arrow	Move to the item on the left hand side
Right arrow	Move to the item on the right hand side
+	Increase the numeric value or make changes
-	Decrease the numeric value or make changes
Page Up key	Move to the next page
Page Dn key	Move to the previous page

Esc key	Main Menu – Quit and do not save changes into CMOS Status Page Setup Menu and Option Page Setup Menu -- Exit current page and return to Main Menu
F1 key	General help, only for Status Page Setup Menu and Option Page Setup Menu
F9 key	Load optimized defaults
F10 key	Save changes and Exit BIOS

Table 5-1: BIOS Navigation Keys

5.1.3 Getting Help

When **F1** is pressed a small help window describing the appropriate keys to use and the possible selections for the highlighted item appears. To exit the Help Window press **Esc** or the **F1** key again.

5.1.4 Unable to Reboot After Configuration Changes

If the computer cannot boot after changes to the system configuration are made, CMOS defaults. Use the jumper described in **Chapter 4**.

5.1.5 BIOS Menu Bar

The **menu bar** on top of the BIOS screen has the following main items:

- **Main** Changes the basic system configuration.
- **Advanced** Changes the advanced system settings.
- **Chipset** Changes the chipset settings
- **Boot** Changes the system boot configuration.
- **Security** Sets User and Supervisor Passwords.
- **Save & Exit** Selects exit options and loads default settings

The following sections completely describe the configuration options found in the menu items at the top of the BIOS screen and listed above.

5.2 Main

The **Main** BIOS menu (**BIOS Menu 1**) appears when the **BIOS Setup** program is entered. The **Main** menu gives an overview of the basic system information.

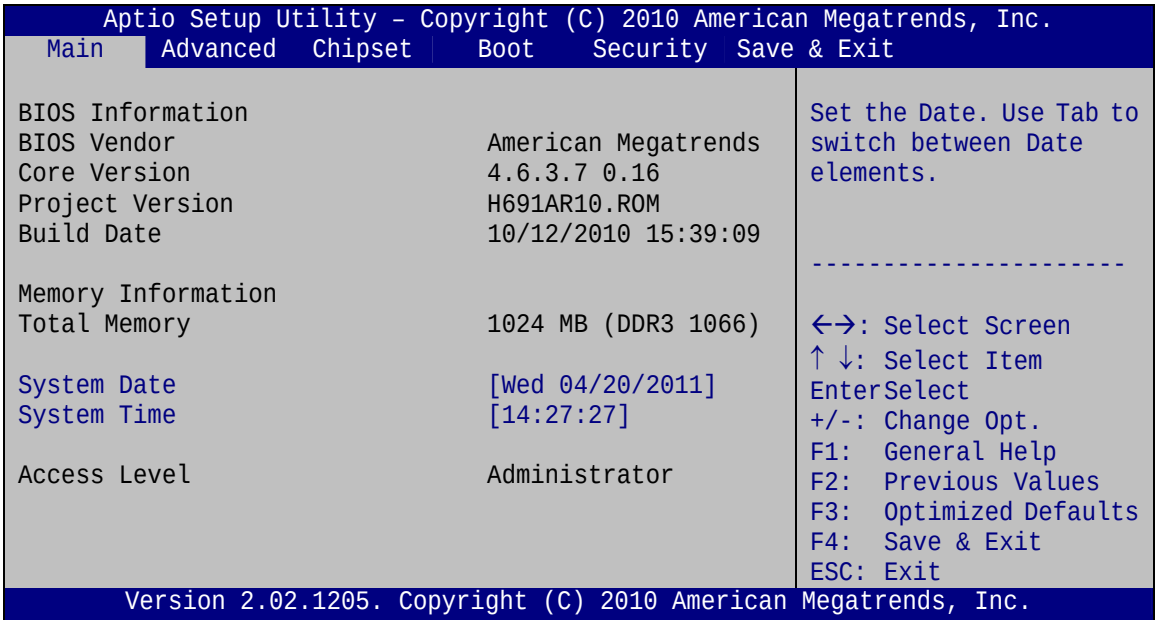
Aptio Setup Utility – Copyright (C) 2010 American Megatrends, Inc.
Main Advanced Chipset Boot Security Save & Exit
BIOS Information
BIOS Vendor American Megatrends
Core Version 4.6.3.7 0.16
Project Version H691AR10.ROM
Build Date 10/12/2010 15:39:09
Memory Information
Total Memory 1024 MB (DDR3 1066)
System Date [Wed 04/20/2011]
System Time [14:27:27]
Access Level Administrator
Set the Date. Use Tab to switch between Date elements.
←→: Select Screen
↑ ↓: Select Item
Enter Select
+/-: Change Opt.
F1: General Help
F2: Previous Values
F3: Optimized Defaults
F4: Save & Exit
ESC: Exit
Version 2.02.1205. Copyright (C) 2010 American Megatrends, Inc.

BIOS Menu 1: Main

➔ System Overview

The **System Overview** lists a brief summary of different system components. The fields in **System Overview** cannot be changed. The items shown in the system overview include:

- **BIOS Vendor:** Installed BIOS vendor
- **Core Version:** Current BIOS version
- **Project Version:** The board version
- **Build Date:** Date the current BIOS version was made
- **Access Level:** User access level

➔ Memory Information

The **Memory Information** lists a brief summary of the on-board memory. The fields in **Memory Information** cannot be changed.

- Total Memory: Displays the auto-detected system memory size and type.

The System Overview field also has two user configurable fields:

➔ **System Date [xx/xx/xx]**

Use the **System Date** option to set the system date. Manually enter the day, month and year.

➔ **System Time [xx:xx:xx]**

Use the **System Time** option to set the system time. Manually enter the hours, minutes and seconds.

5.3 Advanced

Use the **Advanced** menu (**BIOS Menu 2**) to configure the CPU and peripheral devices through the following sub-menus:

WARNING:

Setting the wrong values in the sections below may cause the system to malfunction. Make sure that the settings made are compatible with the hardware.

- ACPI Settings
- Trusted Computing
- CPU Configuration
- SATA Configuration
- USB Configuration
- Super IO Configuration
- H/W Monitor
- Serial Port Console Redirection

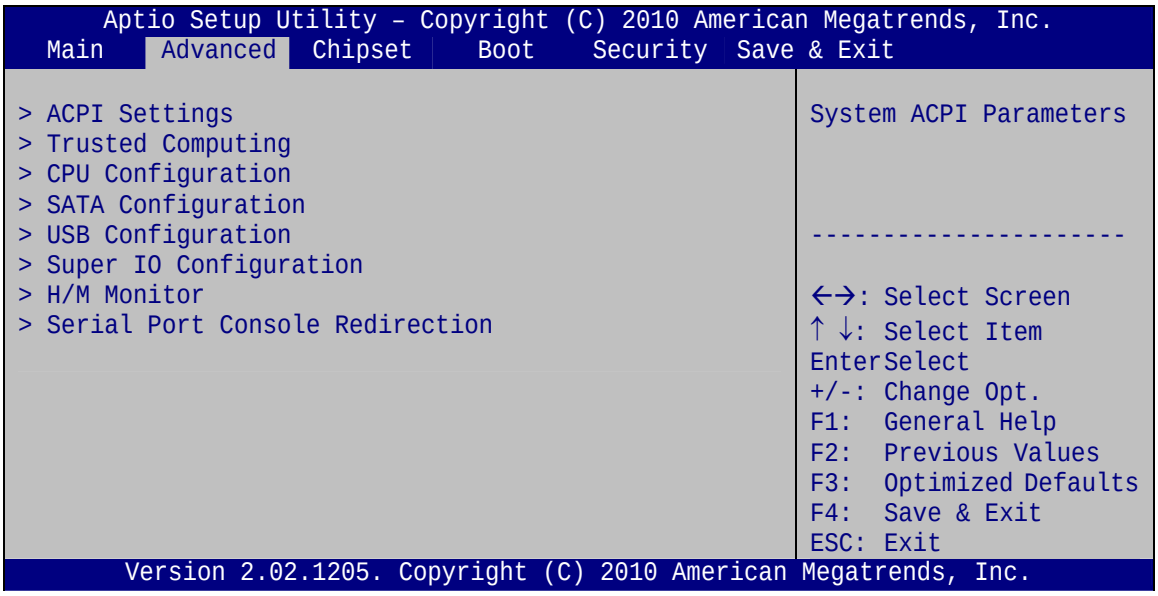

BIOS Menu 2: Advanced

5.3.1 ACPI Settings

The **ACPI Settings** menu (**BIOS Menu 5**) configures the Advanced Configuration and Power Interface (ACPI) options.

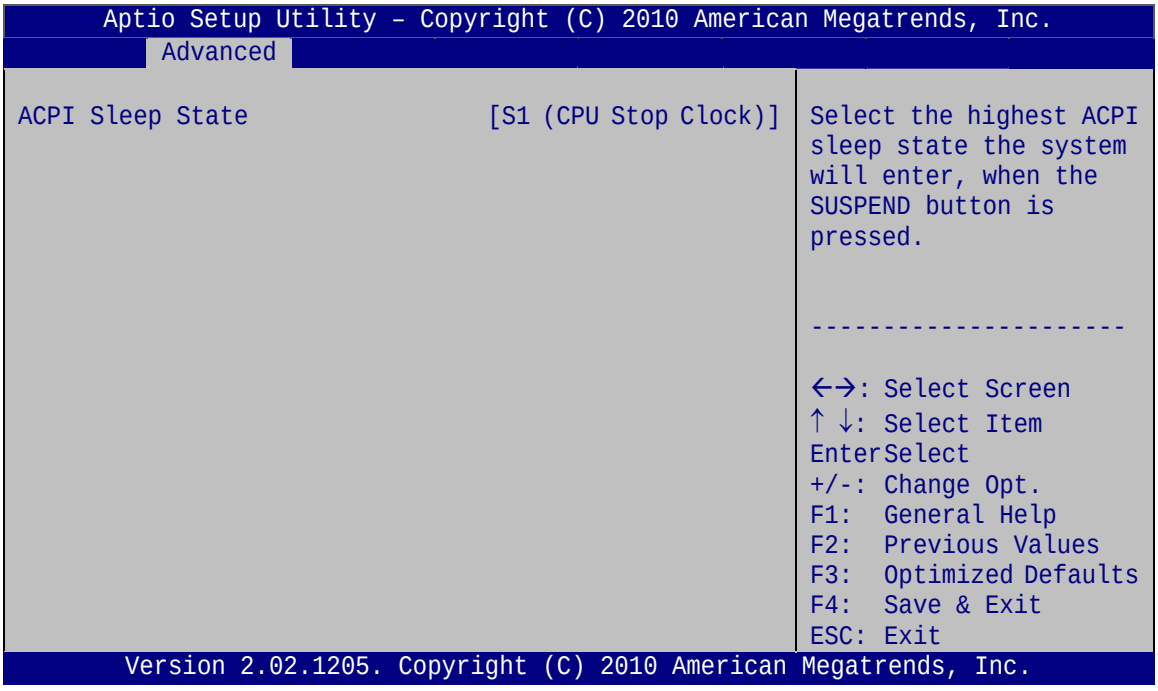
Aptio Setup Utility – Copyright (C) 2010 American Megatrends, Inc.
Advanced
ACPI Sleep State [S1 (CPU Stop Clock)]
Select the highest ACPI sleep state the system will enter, when the SUSPEND button is pressed.

←→: Select Screen
↑ ↓: Select Item
EnterSelect
+/-: Change Opt.
F1: General Help
F2: Previous Values
F3: Optimized Defaults
F4: Save & Exit
ESC: Exit
Version 2.02.1205. Copyright (C) 2010 American Megatrends, Inc.

BIOS Menu 3: ACPI Configuration

➔ **ACPI Sleep State [S3 (CPU Stop Clock)]**

Use the **ACPI Sleep State** option to specify the sleep state the system enters when it is not being used.

➔ **S1 (CPU Stop Clock)** **DEFAULT**	The system enters S1 (POS) sleep state. The system appears off. The CPU is stopped; RAM is refreshed; the system is running in a low power mode.
➔ **S3 (Suspend to RAM)**	The caches are flushed and the CPU is powered off. Power to the RAM is maintained. The computer returns slower to a working state, but more power is saved.

5.3.2 Trusted Computing

Use the **Trusted Computing** menu (**BIOS Menu 4**) to configure settings related to the Trusted Computing Group (TCG) Trusted Platform Module (TPM).

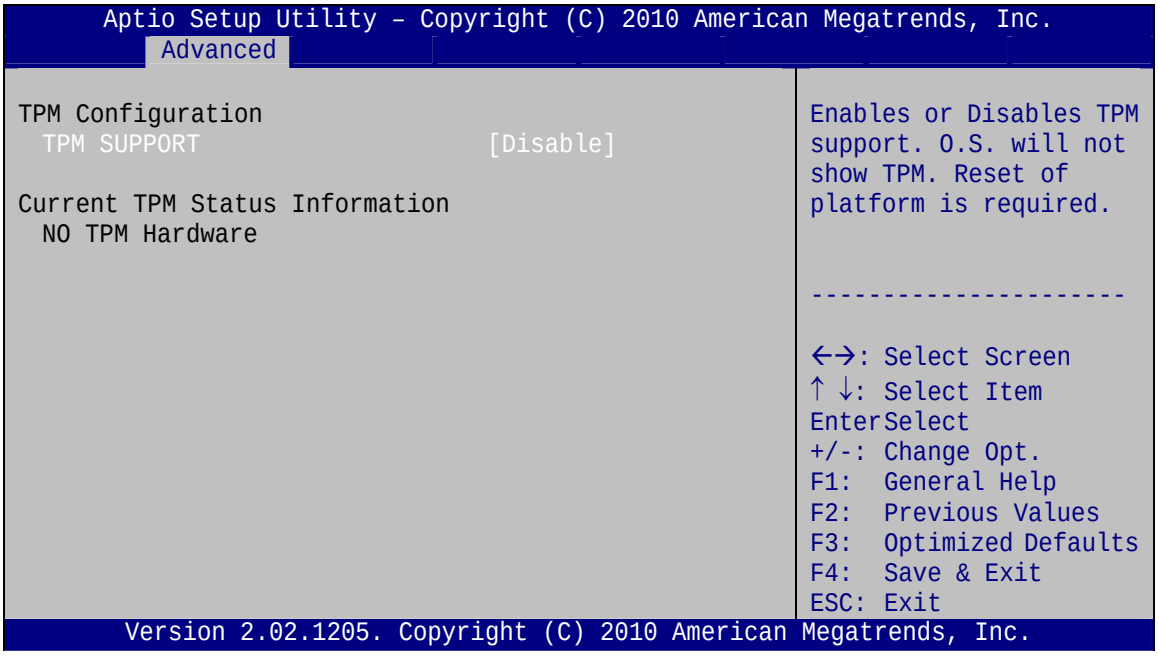
Aptio Setup Utility – Copyright (C) 2010 American Megatrends, Inc.
Advanced
TPM Configuration
TPM SUPPORT [Disable]
Current TPM Status Information
NO TPM Hardware
Enables or Disables TPM support. O.S. will not show TPM. Reset of platform is required.
←→: Select Screen
↑ ↓: Select Item
Enter Select
+/-: Change Opt.
F1: General Help
F2: Previous Values
F3: Optimized Defaults
F4: Save & Exit
ESC: Exit
Version 2.02.1205. Copyright (C) 2010 American Megatrends, Inc.

BIOS Menu 4: TPM Configuration

➔ **TPM Support [Disable]**

Use the **TPM Support** option to configure support for the TPM.

➔ **Disable** **DEFAULT** TPM support is disabled.

➔ **Enable** TPM support is enabled.

5.3.3 CPU Configuration

Use the **CPU Configuration** menu (**BIOS Menu 5**) to view detailed CPU specifications and configure the CPU.

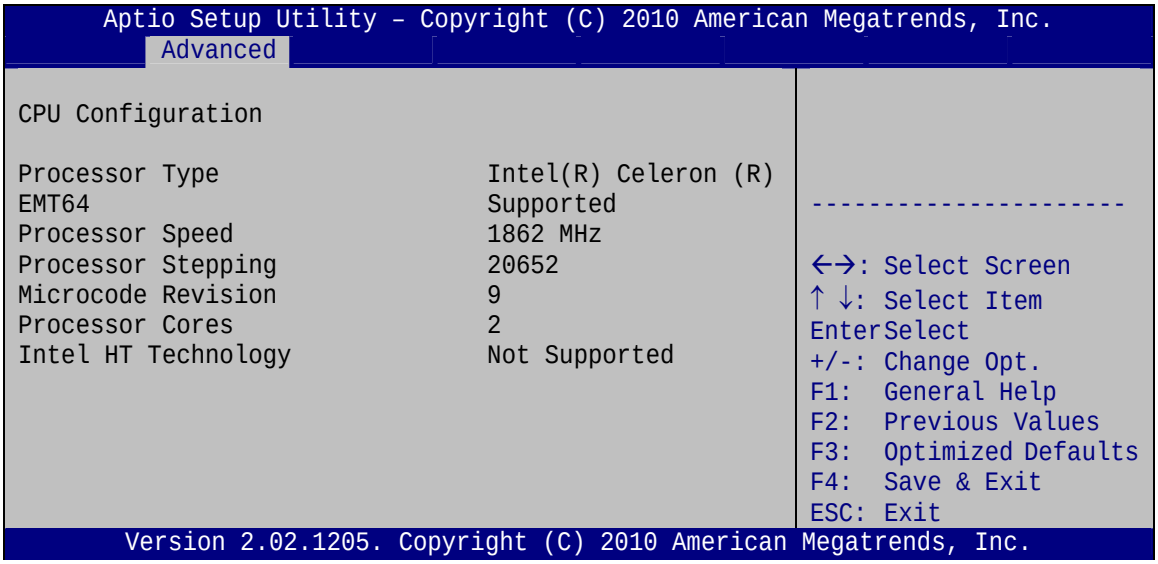

BIOS Menu 5: CPU Configuration

The CPU Configuration menu (**BIOS Menu 5**) lists the following CPU details:

- Processor Type: Lists the brand name of the CPU being used
- EMT64: Indicates if EM64T is supported by the CPU.
- Processor Speed: Lists the CPU processing speed
- Processor Stepping: Lists the CPU processing stepping
- Microcode Revision: Lists the microcode revision
- Processor Cores: Lists the number of the processor core
- Intel HT Technology: Indicates if Intel HT Technology is supported by the CPU.

5.3.4 SATA Configuration

Use the **SATA Configuration** menu (**BIOS Menu 6**) to change and/or set the configuration of the SATA devices installed in the system.

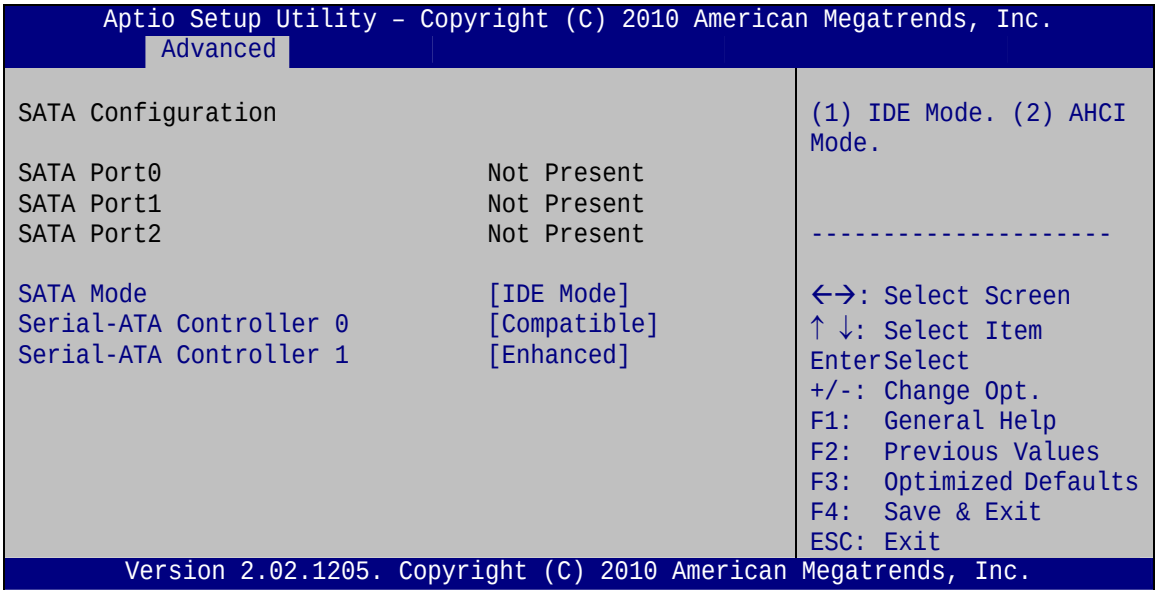

BIOS Menu 6: IDE Configuration

➔ **SATA Mode [IDE Mode]**

Use the **SATA Mode** option to configure SATA devices as normal IDE devices.

➔ **Disable**		Disables SATA devices.
➔ **IDE Mode**	**DEFAULT**	Configures SATA devices as normal IDE device.
➔ **AHCI Mode**		Configures SATA devices as AHCI device.

➔ **Serial-ATA Controller n [Compatible]**

Use the **Serial-ATA Controller** option to configure the SATA controller.

➔ **Disabled**	Disables the on-board SATA controller.
➔ **Enhanced**	Configures the on-board SATA controller to be in Enhanced mode. In this mode, IDE channels and SATA channels are separated.

➔ **Compatible** **DEFAULT** Configures the on-board SATA controller to be in compatible mode. In this mode, a SATA channel will replace one of the IDE channels. This mode supports up to 6 storage devices.

5.3.5 USB Configuration

Use the **USB Configuration** menu (**BIOS Menu 7**) to read USB configuration information and configure the USB settings.

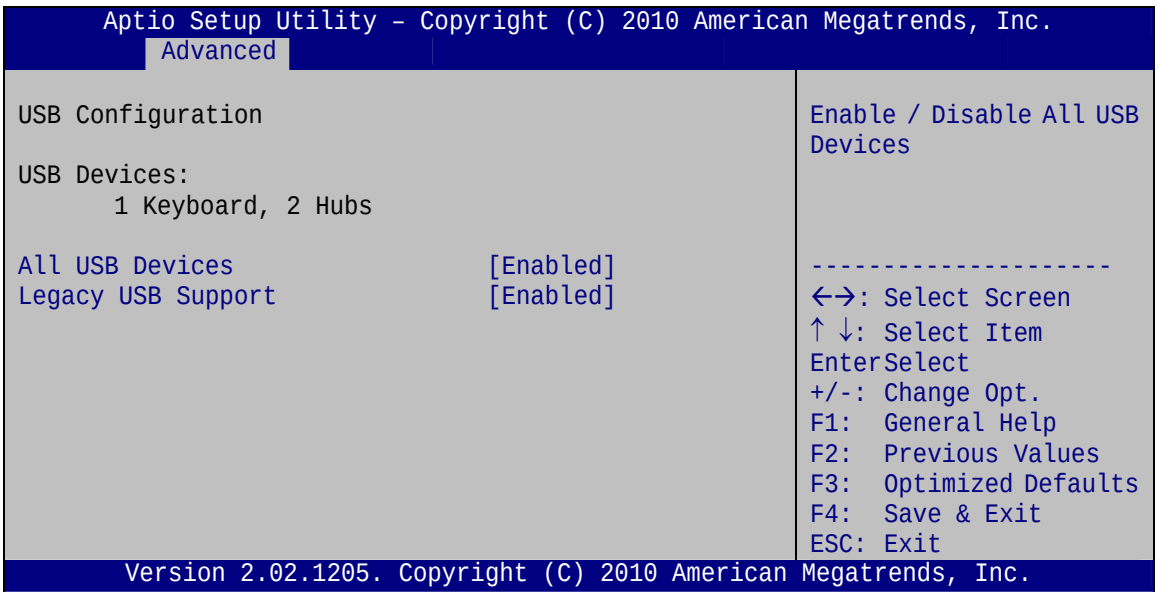

BIOS Menu 7: USB Configuration

➔ **USB Devices**

The **USB Devices Enabled** field lists the USB devices that are enabled on the system

➔ **All USB Devices [Enabled]**

Use this option to enable or disable all USB device support on the system.

➔ **Disabled** All USB device support disabled

➔ **Enabled** **DEFAULT** All USB device support enabled

➔ **Legacy USB Support [Enabled]**

Use the **Legacy USB Support** BIOS option to enable USB mouse and USB keyboard support. Normally if this option is not enabled, any attached USB mouse or USB keyboard does not become available until a USB compatible operating system is fully booted with all USB drivers loaded. When this option is enabled, any attached USB mouse or USB keyboard can control the system even when there is no USB driver loaded onto the system.

➔ **Disabled**		Legacy USB support disabled
➔ **Enabled**	**DEFAULT**	Legacy USB support enabled
➔ **Auto**		Legacy USB support disabled if no USB devices are connected

5.3.6 Super IO Configuration

Use the **Super IO Configuration** menu (**BIOS Menu 8**) to set or change the configurations for the FDD controllers, parallel ports and serial ports.

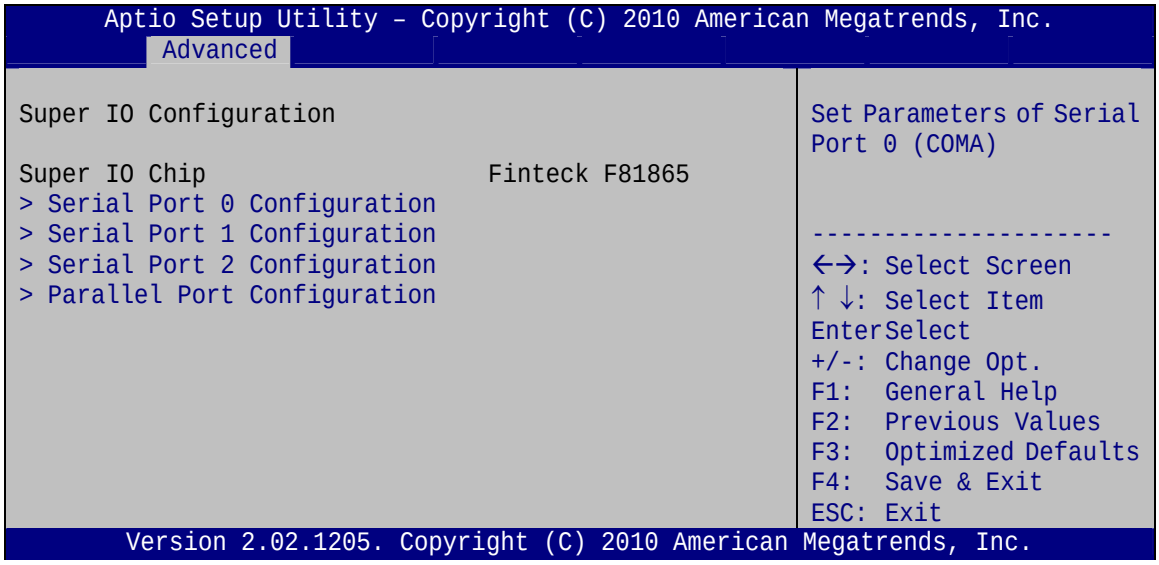
Aptio Setup Utility – Copyright (C) 2010 American Megatrends, Inc.
Advanced
Super IO Configuration
Super IO Chip Finteck F81865
> Serial Port 0 Configuration
> Serial Port 1 Configuration
> Serial Port 2 Configuration
> Parallel Port Configuration
Set Parameters of Serial Port 0 (COMA)
←→: Select Screen
↑ ↓: Select Item
EnterSelect
+/-: Change Opt.
F1: General Help
F2: Previous Values
F3: Optimized Defaults
F4: Save & Exit
ESC: Exit
Version 2.02.1205. Copyright (C) 2010 American Megatrends, Inc.

BIOS Menu 8: Super IO Configuration

5.3.6.1 Serial Port n Configuration

Use the **Serial Port n Configuration** menu (**BIOS Menu 9**) to configure the serial port n.

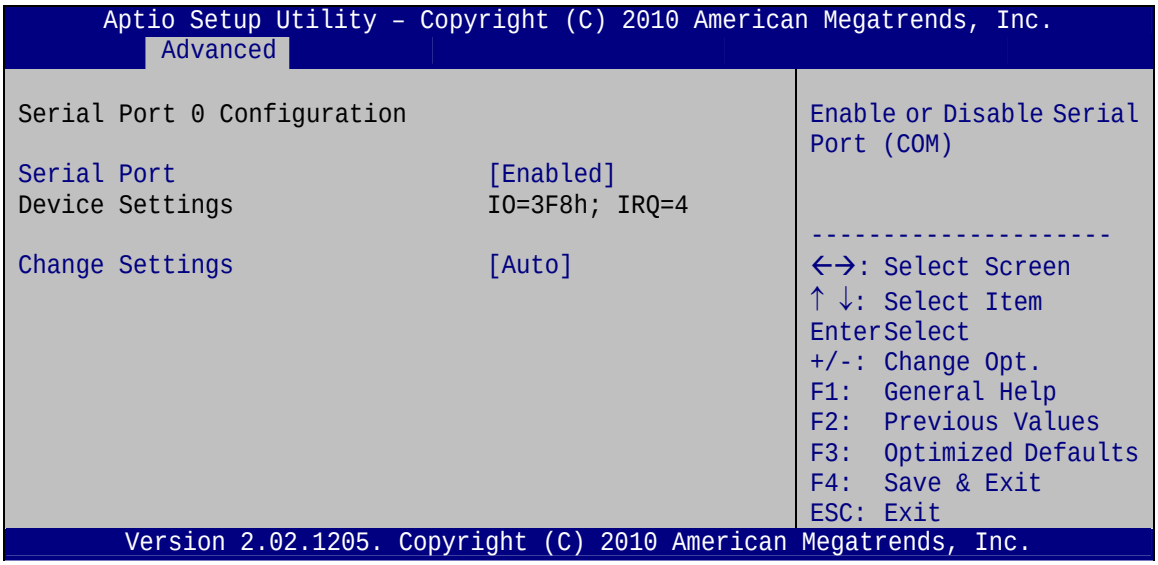

BIOS Menu 9: Serial Port n Configuration Menu

5.3.6.1.1 Serial Port 0 Configuration

➔ **Serial Port [Enabled]**

Use the **Serial Port** option to enable or disable the serial port.

➔ **Disabled**		Disable the serial port
➔ **Enabled**	**DEFAULT**	Enable the serial port

➔ **Change Settings [Auto]**

Use the **Change Settings** option to change the serial port IO port address and interrupt address.

➔ **Auto**	**DEFAULT**	The serial port IO port address and interrupt address are automatically detected.
➔ **IO=3F8h; IRQ=4**		Serial Port I/O port address is 3F8h and the interrupt address is IRQ4

- **IO=3F8h; IRQ=3, 4** — Serial Port I/O port address is 3F8h and the interrupt address is IRQ3, 4
- **IO=2F8h; IRQ=3, 4** — Serial Port I/O port address is 2F8h and the interrupt address is IRQ3, 4
- **IO=2C0h; IRQ=3, 4** — Serial Port I/O port address is 2C0h and the interrupt address is IRQ3, 4
- **IO=2C8h; IRQ=3, 4** — Serial Port I/O port address is 2C8h and the interrupt address is IRQ3, 4

5.3.6.1.2 Serial Port 1 Configuration

➔ **Serial Port [Enabled]**

Use the **Serial Port** option to enable or disable the serial port.

- **Disabled** — Disable the serial port
- **Enabled** DEFAULT — Enable the serial port

➔ **Change Settings [Auto]**

Use the **Change Settings** option to change the serial port IO port address and interrupt address.

- **Auto** DEFAULT — The serial port IO port address and interrupt address are automatically detected.
- **IO=2F8h; IRQ=3** — Serial Port I/O port address is 2F8h and the interrupt address is IRQ3
- **IO=3F8h; IRQ=3, 4** — Serial Port I/O port address is 3F8h and the interrupt address is IRQ3, 4
- **IO=2F8h; IRQ=3, 4** — Serial Port I/O port address is 2F8h and the interrupt address is IRQ3, 4
- **IO=2C0h; IRQ=3, 4** — Serial Port I/O port address is 2C0h and the interrupt address is IRQ3, 4

➔ **IO=2C8h; IRQ=3, 4**		Serial Port I/O port address is 2C8h and the interrupt address is IRQ3, 4

5.3.6.1.3 Serial Port 2 Configuration

➔ **Serial Port [Enabled]**

Use the **Serial Port** option to enable or disable the serial port.

➔ **Disabled**		Disable the serial port
➔ **Enabled**	**DEFAULT**	Enable the serial port

➔ **Change Settings [Auto]**

Use the **Change Settings** option to change the serial port IO port address and interrupt address.

➔ **Auto**	**DEFAULT**	The serial port IO port address and interrupt address are automatically detected.
➔ **IO=3E8h; IRQ=11**		Serial Port I/O port address is 3E8h and the interrupt address is IRQ11
➔ **IO=3E8h; IRQ=10, 11**		Serial Port I/O port address is 3E8h and the interrupt address is IRQ10, 11
➔ **IO=2E8h; IRQ=10, 11**		Serial Port I/O port address is 2E8h and the interrupt address is IRQ10, 11
➔ **IO=2D0h; IRQ=10, 11**		Serial Port I/O port address is 2D0h and the interrupt address is IRQ10, 11
➔ **IO=2D8h; IRQ=10, 11**		Serial Port I/O port address is 2D8h and the interrupt address is IRQ10, 11

5.3.6.1.4 Parallel Port Configuration

➔ **Parallel Port [Enabled]**

Use the **Parallel Port** option to enable or disable the parallel port.

➔ **Disabled**		Disable the parallel port
➔ **Enabled**	**DEFAULT**	Enable the parallel port

➔ **Change Settings [Auto]**

Use the **Change Settings** option to change the parallel port IO port address and interrupt address.

➔ **Auto**	**DEFAULT**	The parallel port IO port address and interrupt address are automatically detected.
➔ **IO=378h; IRQ=7**		Parallel Port I/O port address is 378h and the interrupt address is IRQ7
➔ **IO=278h; IRQ=7**		Parallel Port I/O port address is 278h and the interrupt address is IRQ7
➔ **IO=3BCh; IRQ=7**		Parallel Port I/O port address is 3BCh and the interrupt address is IRQ7
➔ **IO=378h**		Parallel Port I/O port address is 378h
➔ **IO=278h**		Parallel Port I/O port address is 278h
➔ **IO=3BCh**		Parallel Port I/O port address is 3BCh

➔ **Device Mode [Printer Mode]**

Use the **Device Mode** option to select the mode the parallel port operates in. Configuration options are listed below.

- Standard and Bi-direction (SPP) mode **Default**
- EPP-1.9 and SPP Mode
- ECP Mode
- ECP and EPP 1.9 Mode

- Printer mode
- EPP-1.7 and SPP Mode
- ECP and EPP 1.7 Mode

5.3.7 H/W Monitor

The H/W Monitor menu (**BIOS Menu 10**) shows the operating temperature, fan speeds and system voltages.

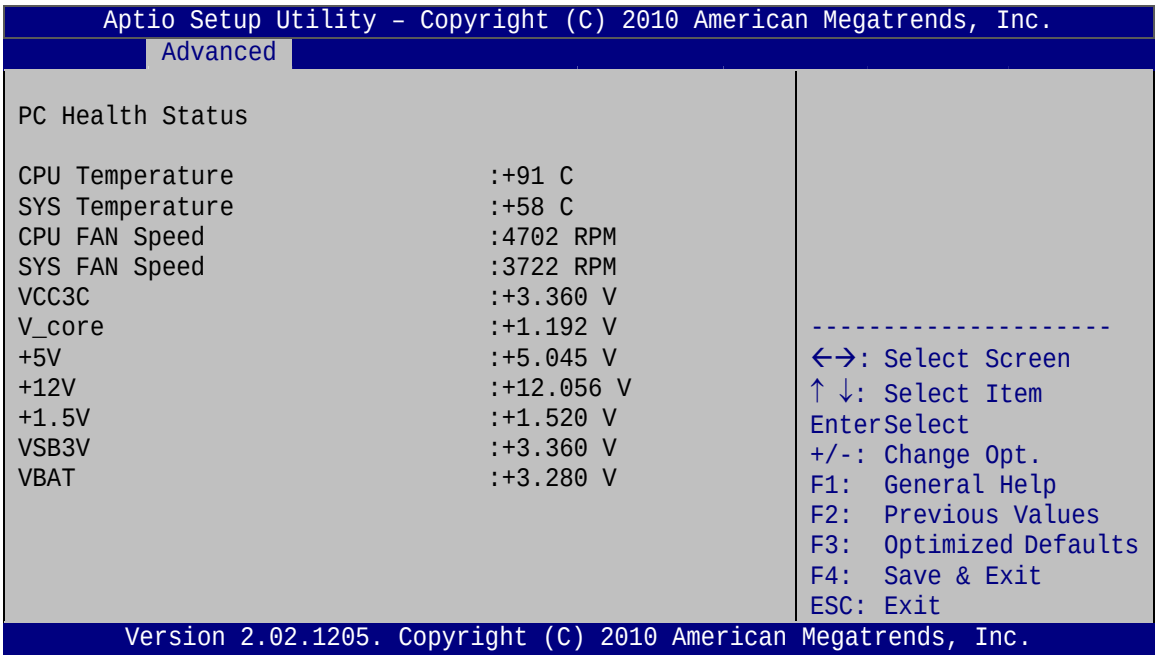

BIOS Menu 10: Hardware Health Configuration

➔ **PC Health Status**

The following system parameters and values are shown. The system parameters that are monitored are:

- System Temperatures:
  - CPU Temperature
  - System Temperature
- Fan Speeds:
  - CPU Fan Speed
  - System Fan Speed
- Voltages:

- VCC3V
- Vcore
- +5V
- +12 V
- +1.5V
- VSB3V
- VBAT

5.3.8 Serial Port Console Redirection

The **Serial Port Console Redirection** menu (**BIOS Menu 11**) allows the console redirection options to be configured. Console redirection allows users to maintain a system remotely by re-directing keyboard input and text output through the serial port.

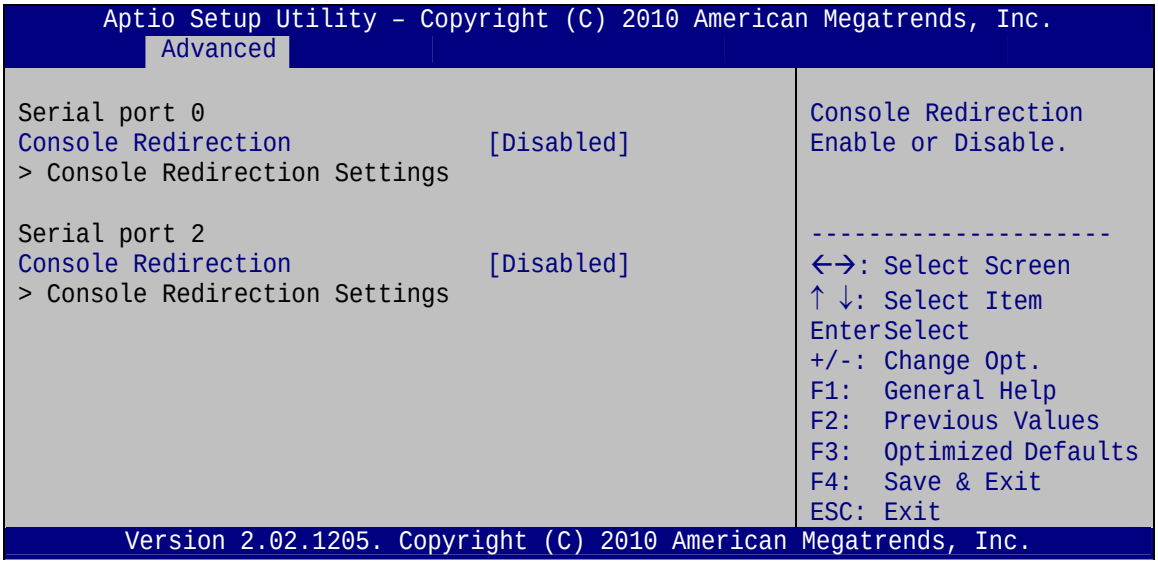

BIOS Menu 11: Serial Port Console Redirection

➔ **Console Redirection [Disabled]**

Use **Console Redirection** option to enable or disable the console redirection function.

➔	**Disabled**	**DEFAULT**	Disabled the console redirection function
➔	**Enabled**		Enabled the console redirection function

5.4 Chipset

Use the **Chipset** menu (**BIOS Menu 12**) to access the Northbridge and Southbridge configuration menus

WARNING!

Setting the wrong values for the Chipset BIOS selections in the Chipset BIOS menu may cause the system to malfunction.

```
      Aptio Setup Utility – Copyright (C) 2010 American Megatrends, Inc.
  Main    Advanced  Chipset    Boot    Security  Save & Exit

> North Bridge                                   North Bridge Parameters
> South Bridge
> Intel IGD SWSCI OpRegion


                                                 ---------------------
                                                 ←→: Select Screen
                                                 ↑ ↓: Select Item
                                                 EnterSelect
                                                 +/-: Change Opt.
                                                 F1:  General Help
                                                 F2:  Previous Values
                                                 F3:  Optimized Defaults
                                                 F4:  Save & Exit
                                                 ESC: Exit

        Version 2.02.1205. Copyright (C) 2010 American Megatrends, Inc.
```

BIOS Menu 12: Chipset

5.4.1 Northbridge Configuration

Use the **Northbridge Chipset Configuration** menu (**BIOS Menu 13**) to configure the Northbridge chipset.

```
Aptio Setup Utility – Copyright (C) 2010 American Megatrends, Inc.
                    Chipset

Memory Information                                IGD Share Memory Size

CPU Type                          Arrandale

Total Memory                      1024 MB (DDR3 1066)

Memory Slot0                      1024 MB (DDR3 1066)
Memory Slot2                         0 MB (DDR3 1066)

                                                    ---------------------
CAS# Latency(tCL)                 7                 ←→: Select Screen
RAS# Active Time(tRAS)            20                ↑ ↓: Select Item
Row Precharge Time(tRP)           7                 EnterSelect
RAS# to CAS# Delay(tRCD)          7                 +/-: Change Opt.
Write Recovery Time(tWR)          8                 F1:  General Help
Row Refresh Cycle Timea(tRFC)     60                F2:  Previous Values
Write to Read Delay(tWTR)         4                 F3:  Optimized Defaults
Active to Active Delay(tRRD)      4                 F4:  Save & Exit
Read CAS# Precharge(tRTP)         5                 ESC: Exit

IGD Memory                        [64M]

Version 2.02.1205. Copyright (C) 2010 American Megatrends, Inc.
```

BIOS Menu 13: Northbridge Chipset Configuration

➔ **IGD Memory [32 MB]**

Use the **IGD Memory** option to specify the amount of system memory that can be used by the Internal graphics device.

➔ **Disable**		
➔ **32 MB**	**DEFAULT**	32 MB of memory used by internal graphics device
➔ **64 MB**		64 MB of memory used by internal graphics device

5.4.2 Southbridge Configuration

Use the **Southbridge Configuration** menu (**BIOS Menu 14**) to configure the Southbridge chipset.

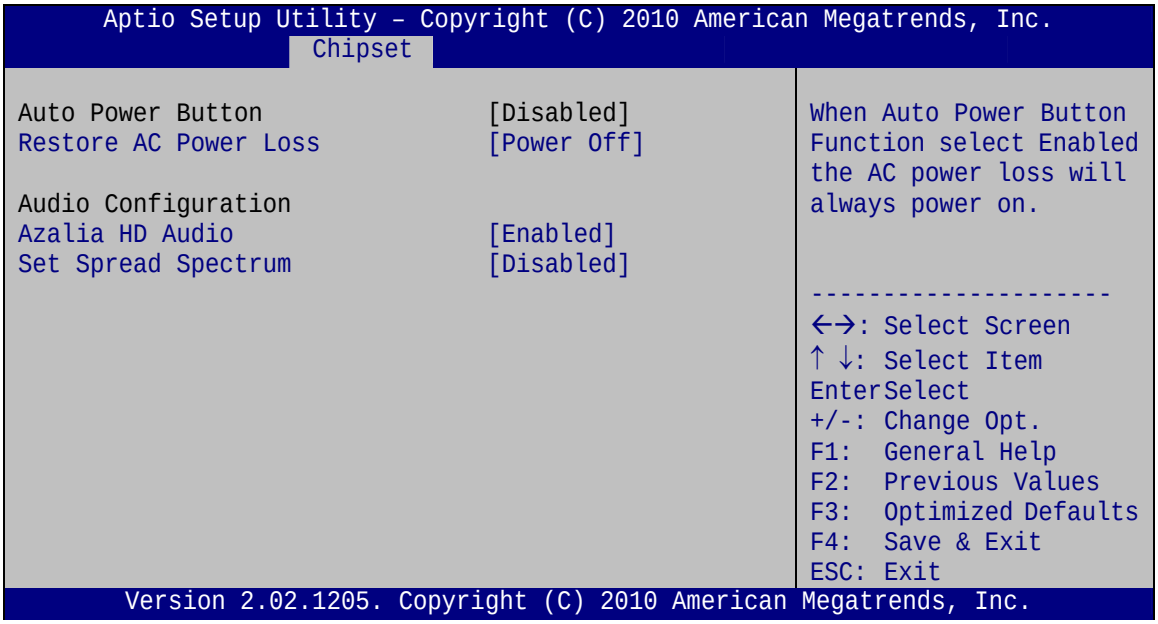
Aptio Setup Utility – Copyright (C) 2010 American Megatrends, Inc.
Chipset
Auto Power Button [Disabled]
Restore AC Power Loss [Power Off]
Audio Configuration
Azalia HD Audio [Enabled]
Set Spread Spectrum [Disabled]
When Auto Power Button Function select Enabled the AC power loss will always power on.
←→: Select Screen
↑ ↓: Select Item
Enter Select
+/-: Change Opt.
F1: General Help
F2: Previous Values
F3: Optimized Defaults
F4: Save & Exit
ESC: Exit
Version 2.02.1205. Copyright (C) 2010 American Megatrends, Inc.

BIOS Menu 14: Southbridge Chipset Configuration

➔ **Restore on AC Power Loss [Power Off]**

Use the **Restore on AC Power Loss** BIOS option to specify what state the system returns to if there is a sudden loss of power to the system.

➔ **Power Off**	**DEFAULT**	The system remains turned off
➔ **Power On**		The system turns on
➔ **Last State**		The system returns to its previous state. If it was on, it turns itself on. If it was off, it remains off.

➔ **Azalia HD Audio [Enabled]**

Use the **Azalia HD Audio** option to enable or disable the High Definition Audio controller.

➔ **Disabled**	The onboard High Definition Audio controller is disabled

➔ **Enabled** **DEFAULT** The onboard High Definition Audio controller automatically detected and enabled

➔ **Set Spread Spectrum [Disabled]**

Use the **Set Spread Spectrum** option to enable or disable the Set Spread Spectrum function.

➔ **Disabled** **DEFAULT** Set Spread Spectrum is disabled

➔ **Enabled** Set Spread Spectrum is enabled

5.4.3 Intel IGD SWSCI OpRegion

Use the **Intel IGD SWSCI OpRegion** menu (**BIOS Menu 15**) to configure the video device connected to the system.

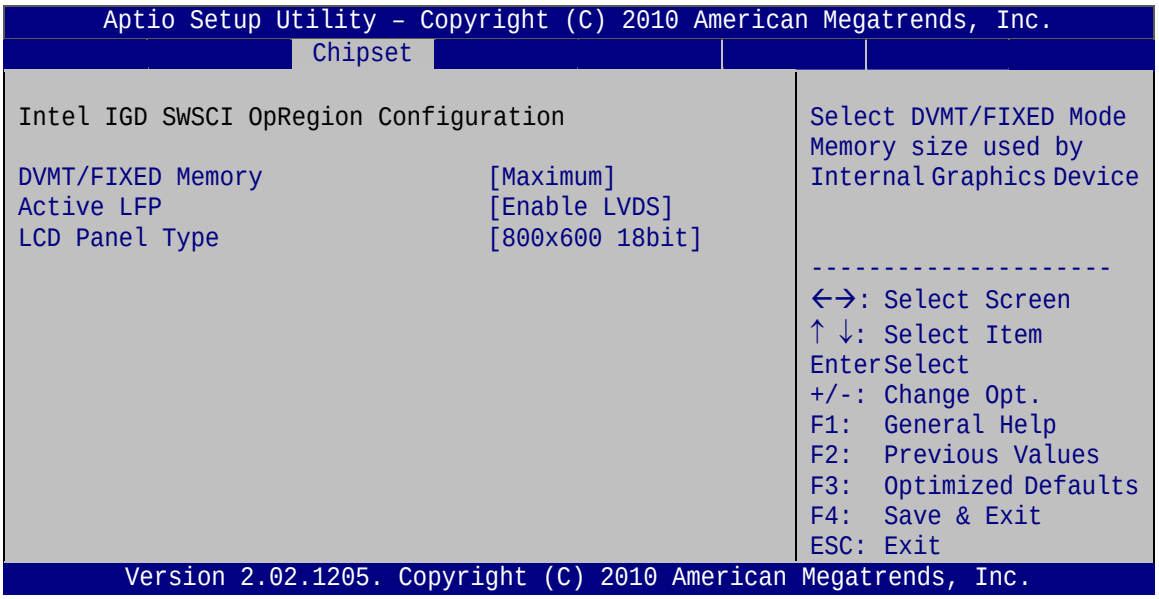
Aptio Setup Utility – Copyright (C) 2010 American Megatrends, Inc.
Chipset
Intel IGD SWSCI OpRegion Configuration
DVMT/FIXED Memory [Maximum]
Active LFP [Enable LVDS]
LCD Panel Type [800x600 18bit]
Select DVMT/FIXED Mode Memory size used by Internal Graphics Device
←→: Select Screen
↑ ↓: Select Item
Enter Select
+/-: Change Opt.
F1: General Help
F2: Previous Values
F3: Optimized Defaults
F4: Save & Exit
ESC: Exit
Version 2.02.1205. Copyright (C) 2010 American Megatrends, Inc.

BIOS Menu 15: Intel IGD SWSCI OpRegion

➔ **DVMT/FIXED Memory [Maximum]**

Use the **DVMT/FIXED Memory** option to specify the maximum amount of memory that can be allocated as graphics memory. Configuration options are listed below.

- 128 MB

- 256 MB
- Maximum **Default**

➔ **Active LFP [Enable LVDS]**

Use the **Active LFP** option to enable or disable LVDS.

➔ **Disable LVDS** **DEFAULT** LVDS is disabled

➔ **Enable LVDS** LVDS is enabled

➔ **LCD Panel Type [Select by Panel ID]**

Use the **LCD Panel Type** option to select the type of flat panel connected to the system. Configuration options are listed below.

- Select by Panel ID **DEFAULT**
- 800x600 18bit
- 1024x768 18bit
- 1024x768 24bit
- 1280x800 18bit
- 1366x768 18bit
- 1400x1050 48bit
- 1440x900 48bit
- 1600x900 48bit
- 1600x1200 48bit
- 1680x1050 48bit
- 1920x1080 48bit
- 1920x1200 48bit
- 2048x1536 48bit

5.5 Boot

Use the **Boot** menu (**BIOS Menu 16**) to configure system boot options.

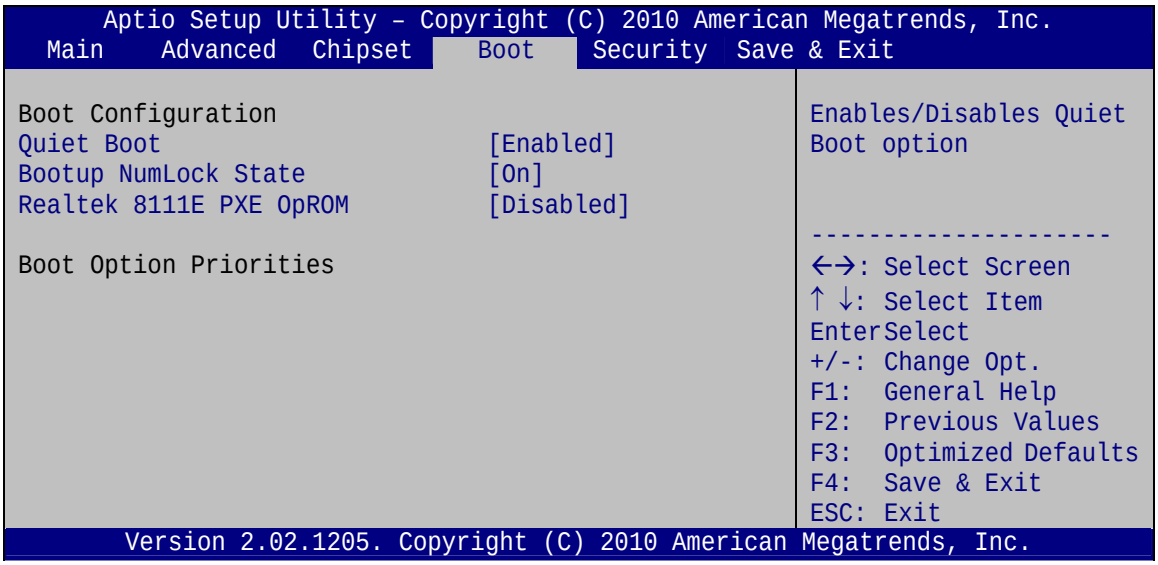
Aptio Setup Utility – Copyright (C) 2010 American Megatrends, Inc.
Main Advanced Chipset Boot Security Save & Exit
Boot Configuration
Quiet Boot [Enabled]
Bootup NumLock State [On]
Realtek 8111E PXE OpROM [Disabled]
Boot Option Priorities
Enables/Disables Quiet Boot option
←→: Select Screen
↑ ↓: Select Item
EnterSelect
+/-: Change Opt.
F1: General Help
F2: Previous Values
F3: Optimized Defaults
F4: Save & Exit
ESC: Exit
Version 2.02.1205. Copyright (C) 2010 American Megatrends, Inc.

BIOS Menu 16: Boot

➔ **Quiet Boot [Enabled]**

Use the **Quiet Boot** BIOS option to select the screen display when the system boots.

➔ **Disabled** Normal POST messages displayed

➔ **Enabled** **DEFAULT** OEM Logo displayed instead of POST messages

➔ **Bootup NumLock State [On]**

Use the **Bootup NumLock State** BIOS option to specify if the number lock setting must be modified during boot up.

➔ **On** **DEFAULT** Allows the Number Lock on the keyboard to be enabled automatically when the computer system boots up. This allows the immediate use of the 10-key numeric keypad located on the right side of the keyboard. To confirm this, the Number Lock LED light on the keyboard is lit.

➔ **Off** Does not enable the keyboard Number Lock automatically. To use the 10-keys on the keyboard, press the Number Lock key located on the upper left-hand corner of the 10-key pad. The Number Lock LED on the keyboard lights up when the Number Lock is engaged.

➔ **Realtek 8111E PXE OpROM [Disabled]**

Use the **Realtek 8111E PXE OpROM** BIOS option to enable or disable Boot Option for Legacy Network Devices.

➔ **Disabled** **DEFAULT** Disables Boot Option for Legacy Network Devices.

➔ **Enabled** Enables Boot Option for Legacy Network Devices.

5.6 Security

Use the **Security** menu (**BIOS Menu 17**) to set system and user passwords.

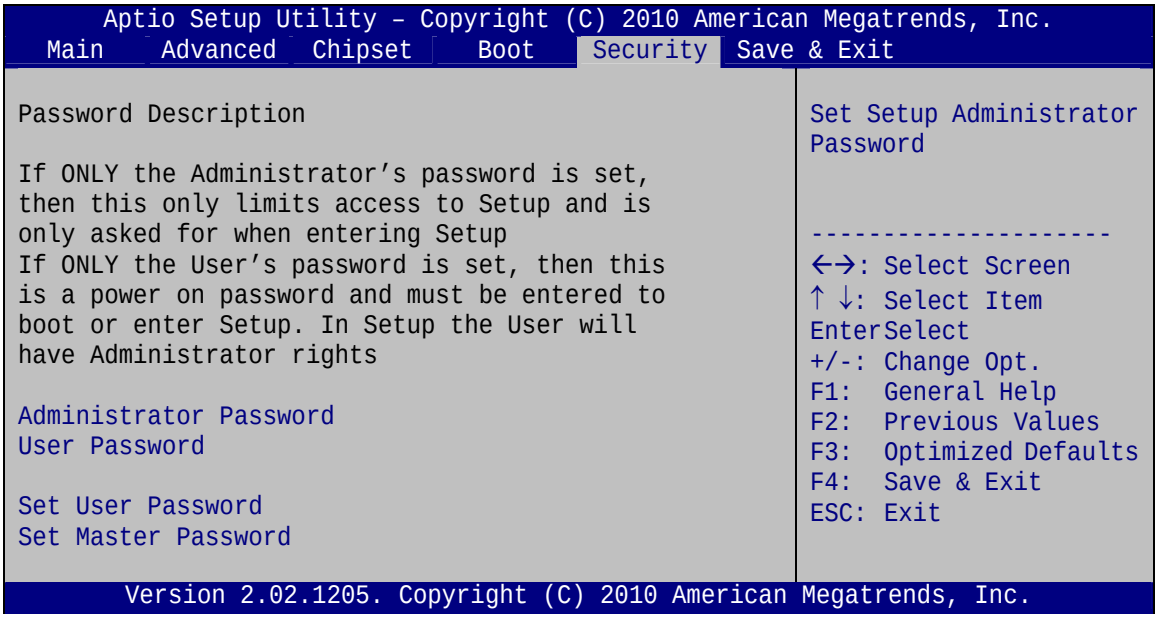
Aptio Setup Utility – Copyright (C) 2010 American Megatrends, Inc.
Main Advanced Chipset Boot Security Save & Exit
Password Description
If ONLY the Administrator's password is set, then this only limits access to Setup and is only asked for when entering Setup
If ONLY the User's password is set, then this is a power on password and must be entered to boot or enter Setup. In Setup the User will have Administrator rights
Administrator Password
User Password
Set User Password
Set Master Password
Set Setup Administrator Password
←→: Select Screen
↑ ↓: Select Item
Enter Select
+/-: Change Opt.
F1: General Help
F2: Previous Values
F3: Optimized Defaults
F4: Save & Exit
ESC: Exit
Version 2.02.1205. Copyright (C) 2010 American Megatrends, Inc.

BIOS Menu 17: Security

➔ **Administrator Password**

Use the **Administrator Password** field to set or change a administrator password.

➔ **User Password**

Use the **User Password** field to set or change a user password.

➔ **Set User Password**

Use the **Set User Password** field to set or change an HDD user password.

NOTE:

It is recommended that the system be reset after setting a new HDD password.

5.7 Exit

Use the **Exit** menu (**BIOS Menu 18**) to load default BIOS values, optimal failsafe values and to save configuration changes.

```
     Aptio Setup Utility – Copyright (C) 2010 American Megatrends, Inc.
 Main    Advanced   Chipset    Boot    Security  Save & Exit

 Save Changes and Reset                    Reset the system after
 Discard Changes and Reset                 saving the changes.

 Restore Defaults
 Save as User Defaults
 Restore User Defaults                     ---------------------
                                           ←→: Select Screen
                                           ↑ ↓: Select Item
                                           EnterSelect
                                           +/-: Change Opt.
                                           F1:  General Help
                                           F2:  Previous Values
                                           F3:  Optimized Defaults
                                           F4:  Save & Exit
                                           ESC: Exit
       Version 2.02.1205. Copyright (C) 2010 American Megatrends, Inc.
```

BIOS Menu 18: Exit

➔ **Save Changes and Reset**

Use the **Save Changes and Reset** option to save the changes made to the BIOS options and reset the system.

➔ **Discard Changes and Reset**

Use the **Discard Changes and Reset** option to exit the system without saving the changes made to the BIOS configuration setup program.

➔ **Restore Defaults**

Use the **Restore Defaults** option to load the optimal default values for each of the parameters on the Setup menus. **F3 key can be used for this operation.**

➔ **Save as User Defaults**

Use the **Save as User Defaults** option to save the changes done so far as user defaults.

➔ **Restore User Defaults**

Use the **Restore User Defaults** option to restore the user defaults to all the setup options.

Chapter

6

Software Drivers

6.1 Available Software Drivers

NOTE:

The content of the CD may vary throughout the life cycle of the product and is subject to change without prior notice. Visit the PACSmate website or contact technical support for the latest updates.

The following drivers can be installed on the system:

- Chipset
- VGA
- LAN
- Audio
- Touch screen
- Wireless
- Keypad function

Installation instructions are given below.

6.2 Chipset Driver Installation

To install the chipset driver, please do the following.

Step 1: Access the driver list from the driver CD.

Step 2: Click **Chipset** and locate the install icon "**infinst_autol_9_1_1_1024.exe**". Double click the install icon.

Step 3: The setup files are extracted as shown in **Figure 6-1**.

Figure 6-1: Chipset Driver File Extraction Screen

Step 4: When the setup files are completely extracted the **Welcome Screen** in **Figure 6-2** appears.

Step 5: Click **NEXT** to continue.

Intel® Chipset Device Software
Intel® Chipset Device Software
Welcome to the Setup Program
This setup program will install the Intel® Chipset Device Software onto this computer. It is strongly recommended that you exit all programs before continuing.
< Back
Next >
Cancel
Intel® Installation Framework

Figure 6-2: Chipset Driver Welcome Screen

Step 6: The license agreement in **Figure 6-3** appears.

Step 7: Read the **License Agreement** and click **YES** to continue.

Intel® Chipset Device Software
Intel® Chipset Device Software
License Agreement
intel
You must accept all of the terms of the license agreement in order to continue the setup program. Do you accept the terms?
INTEL SOFTWARE LICENSE AGREEMENT (OEM / IHV / ISV Distribution & Single User)
IMPORTANT - READ BEFORE COPYING, INSTALLING OR USING.
Do not use or load this software and any associated materials (collectively, the "Software") until you have carefully read the following terms and conditions. By loading or using the Software, you agree to the terms of this Agreement. If you do not wish to so agree, do not install or use the Software.
Please Also Note:
* If you are an Original Equipment Manufacturer (OEM), Independent Hardware Vendor (IHV), or Independent Software Vendor (ISV), this complete LICENSE AGREEMENT applies;
< Back
Yes
No
Intel® Installation Framework

Figure 6-3: Chipset Driver License Agreement

Step 8: The **Readme File Information** screen in **Figure 6-4** appears.

Step 9: Click **NEXT** to continue.

Intel® Chipset Device Software
Intel® Chipset Device Software
Readme File Information
Refer to the Readme file below to view the system requirements and installation information.
Press the Page Down key to view the rest of the file.
****
* Product: Intel(R) Chipset Device Software
* Release: Production Version
* Version: 9.0.0.1008
* Target Chipset#: Intel(R) 4 Series Chipset
* Date: May 01 2008
****
< Back
Next >
Cancel
Intel® Installation Framework

Figure 6-4: Readme File Information Screen

Step 10: Setup operations are performed as shown in **Figure 6-5**.

Step 11: Once the setup operations are complete, click **NEXT** to continue.

Intel® Chipset Device Software
Intel® Chipset Device Software
Setup Progress
Please wait while the following setup operations are performed:
Installing Driver: Intel(R) 82801G (ICH7 Family) USB Universal Host Controller - 27C9
Version: 8.2.0.1008
Installing Driver: Intel(R) 82801G (ICH7 Family) USB Universal Host Controller - 27CA
Version: 8.2.0.1008
Installing Driver: Intel(R) 82801G (ICH7 Family) USB Universal Host Controller - 27CB
Version: 8.2.0.1008
Installing Driver: Intel(R) 82801G (ICH7 Family) USB2 Enhanced Host Controller - 27CC
Version: 8.2.0.1008
Click Next to continue.
Next
Intel® Installation Framework

Figure 6-5: Setup Progress Screen

Step 12: The **Setup Is Complete** screen appears.

Step 13: Select "**Yes, I want to restart the computer now**" and click **Finish** (**Figure 6-6)**.

Intel® Chipset Device Software
Intel® Chipset Device Software
Setup Is Complete
intel
You must restart this computer for the changes to take effect. Would you like to restart the computer now?
Yes, I want to restart this computer now.
No, I will restart this computer later.
Click Finish, then remove any installation media from the drives.
Finish
Intel® Installation Framework

Figure 6-6: Chipset Driver Installation Finish Screen

6.3 VGA Driver Installation

To install the VGA driver, please do the following.

Step 1: Access the driver list from the driver CD

Step 2: Click **VGA** and double click on the folder which corresponds to your operating system.

Step 3: Double click on the install icon.

Step 4: The **VGA Readme File** in **Figure 6-7** appears.

Step 5: Click **NEXT** to continue.

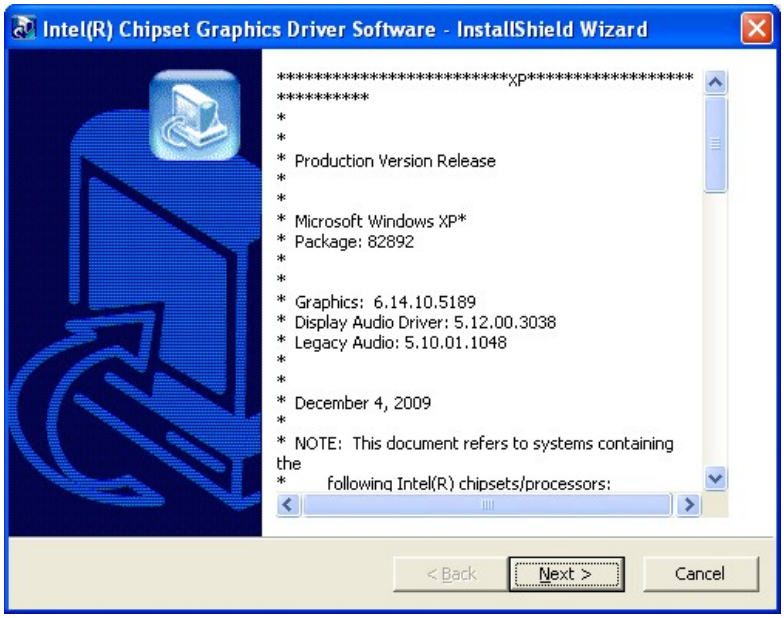

Figure 6-7: VGA Driver Readme File

Step 6: The installation files are extracted as shown in **Figure 6-8**.

Step 7: Click **NEXT** to continue.

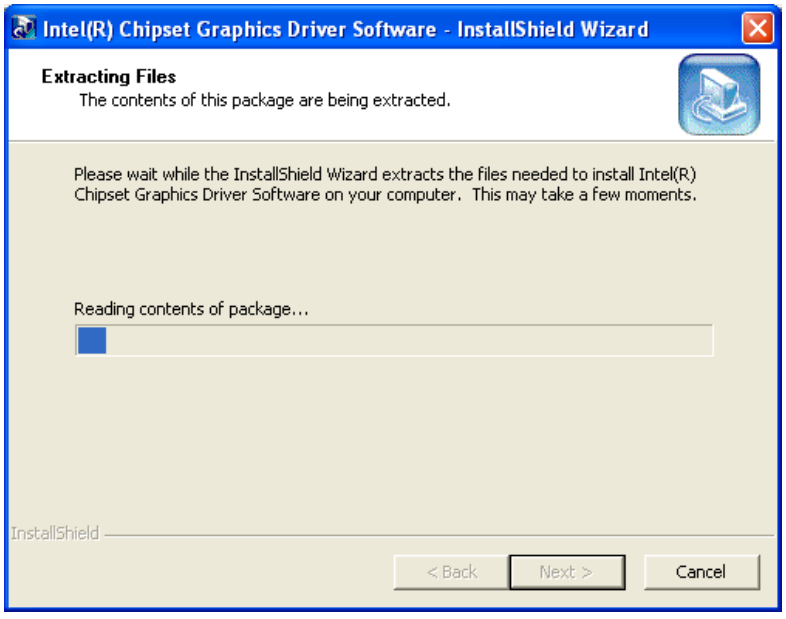
Intel(R) Chipset Graphics Driver Software - InstallShield Wizard
Extracting Files
The contents of this package are being extracted.
Please wait while the InstallShield Wizard extracts the files needed to install Intel(R) Chipset Graphics Driver Software on your computer. This may take a few moments.
Reading contents of package...
InstallShield
< Back
Next >
Cancel

Figure 6-8: VGA Driver Setup File Extraction Screen

Step 8: The **Welcome Screen** in **Figure 6-9** appears.

Step 9: Click **NEXT** to continue.

Intel® Graphics Media Accelerator Driver
Intel® Graphics Media Accelerator Driver
Welcome to the Setup Program
This setup program will install the Intel® Graphics Media Accelerator Driver onto this computer. It is strongly recommended that you exit all programs before continuing. Click Next to continue.
< Back
Next >
Cancel
Intel® Installation Framework

Figure 6-9: VGA Driver Welcome Screen

Step 10: The **License Agreement** in **Figure 6-10** appears.

Step 11: Click **YES** to accept and continue.

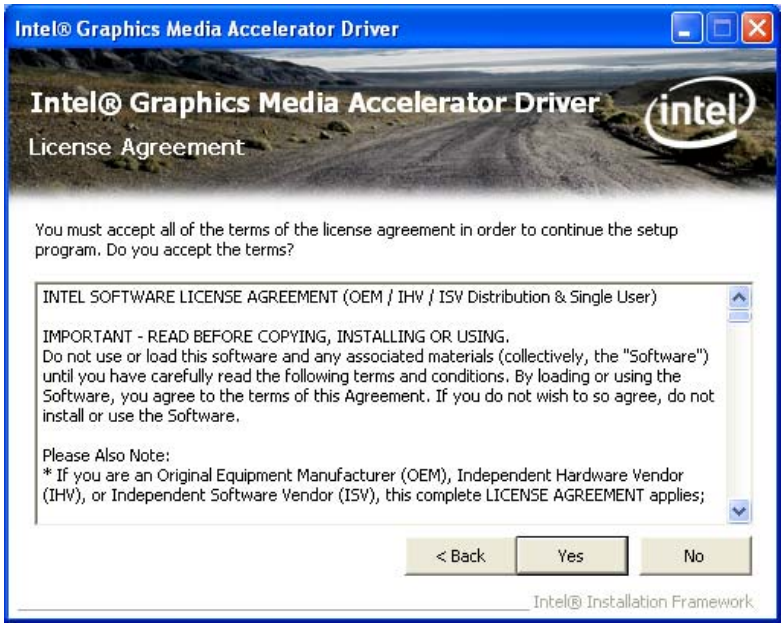
Intel® Graphics Media Accelerator Driver
Intel® Graphics Media Accelerator Driver
License Agreement
You must accept all of the terms of the license agreement in order to continue the setup program. Do you accept the terms?
INTEL SOFTWARE LICENSE AGREEMENT (OEM / IHV / ISV Distribution & Single User)
IMPORTANT - READ BEFORE COPYING, INSTALLING OR USING.
Do not use or load this software and any associated materials (collectively, the "Software") until you have carefully read the following terms and conditions. By loading or using the Software, you agree to the terms of this Agreement. If you do not wish to so agree, do not install or use the Software.
Please Also Note:
* If you are an Original Equipment Manufacturer (OEM), Independent Hardware Vendor (IHV), or Independent Software Vendor (ISV), this complete LICENSE AGREEMENT applies;
< Back
Yes
No
Intel® Installation Framework

Figure 6-10: VGA Driver License Agreement

Step 12: The **Readme File** in **Figure 6-11** appears.

Step 13: Click **NEXT** to continue.

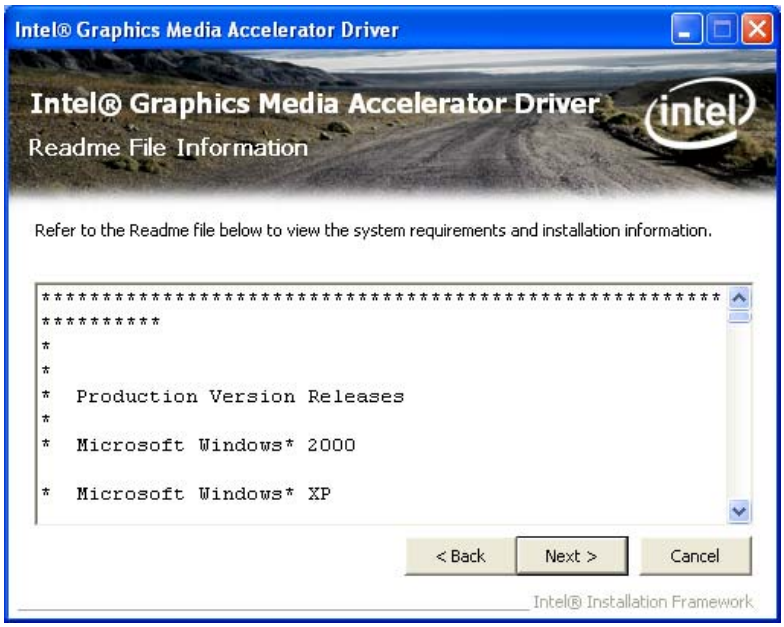

Figure 6-11: VGA Driver Readme File

Step 14: Setup operations are performed as shown in **Figure 6-12**.

Step 15: Once the setup operations are complete, click **NEXT** to continue.

Figure 6-12: VGA Driver Setup Operations

Step 16: The **Setup Is Complete** screen appears.

Step 17: Select "**Yes, I want to restart the computer now**" and click **FINISH**. See **Figure 6-13**.

Intel® Graphics Media Accelerator Driver
Intel® Graphics Media Accelerator Driver
Setup Is Complete
intel
You must restart this computer for the changes to take effect. Would you like to restart the computer now?
Yes, I want to restart this computer now.
No, I will restart this computer later.
Click Finish, then remove any installation media from the drives.
Finish
Intel® Installation Framework

Figure 6-13: VGA Driver Setup Is Complete Screen

6.4 LAN Driver Installation

To install the LAN driver, please do the following.

Step 1: Access the driver list from the driver CD

Step 2: Locate the installation icon **setup.exe** and double click on it.

Step 3: The **Welcome** screen in **Figure 6-14** appears.

Step 4: Click **NEXT** to continue.

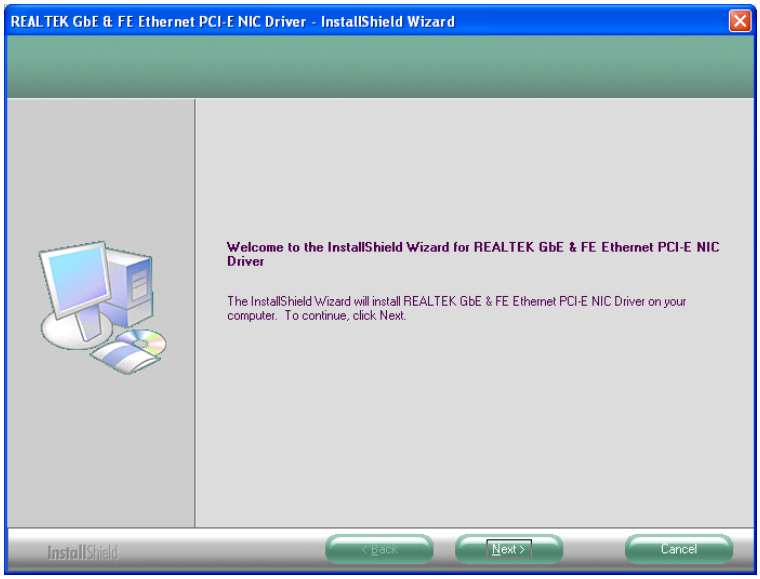
REALTEK GbE & FE Ethernet PCI-E NIC Driver - InstallShield Wizard
Welcome to the InstallShield Wizard for REALTEK GbE & FE Ethernet PCI-E NIC Driver
The InstallShield Wizard will install REALTEK GbE & FE Ethernet PCI-E NIC Driver on your computer. To continue, click Next.
InstallShield
< Back
Next >
Cancel

Figure 6-14: LAN Driver Welcome Screen

Step 5: The **Ready to Install** screen in **Figure 6-15** appears.

Step 6: Click **INSTALL** to proceed with the installation.

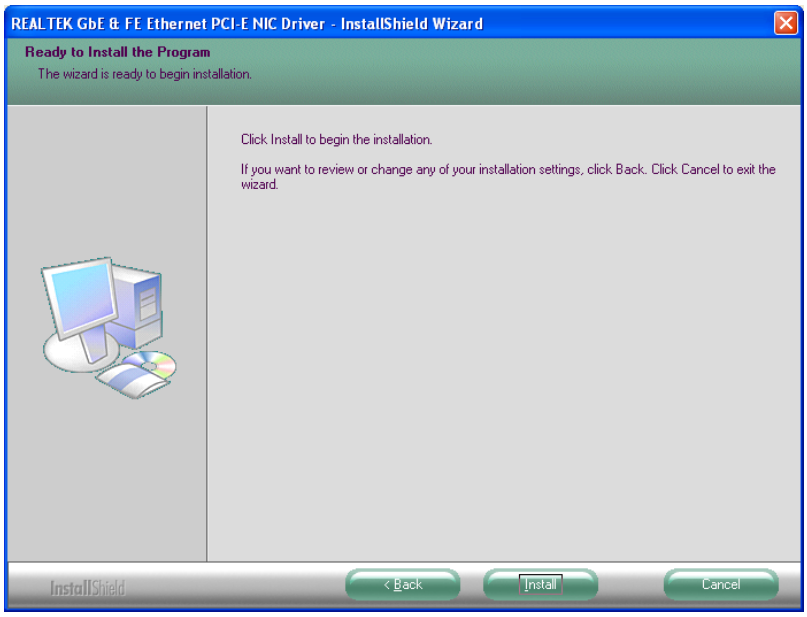
REALTEK GbE & FE Ethernet PCI-E NIC Driver - InstallShield Wizard
Ready to Install the Program
The wizard is ready to begin installation.
Click Install to begin the installation.
If you want to review or change any of your installation settings, click Back. Click Cancel to exit the wizard.
InstallShield
< Back
Install
Cancel

Figure 6-15: LAN Driver Welcome Screen

Step 7: The program begins to install.

Step 8: The installation progress can be monitored in the progress bar shown in **Figure**

6-16.

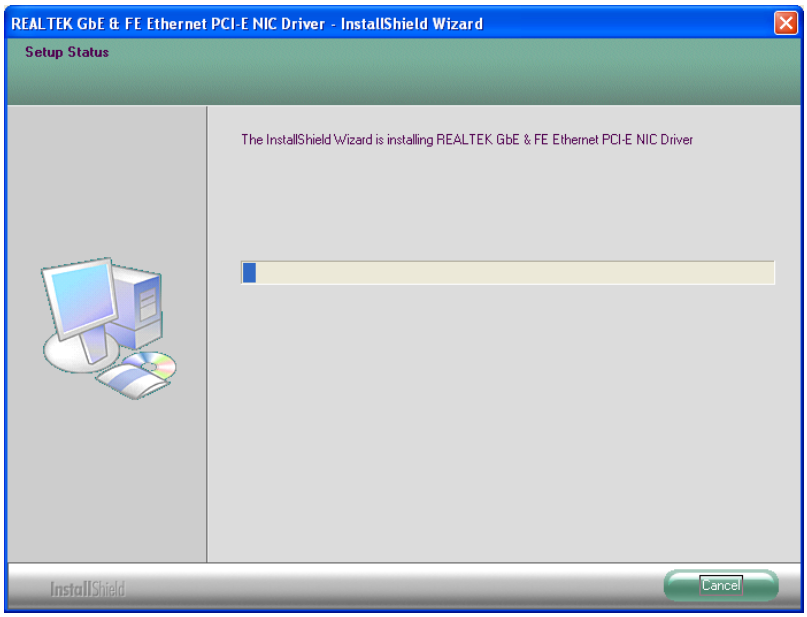
REALTEK GbE & FE Ethernet PCI-E NIC Driver - InstallShield Wizard
Setup Status
The InstallShield Wizard is installing REALTEK GbE & FE Ethernet PCI-E NIC Driver
InstallShield
Cancel

Figure 6-16: LAN Driver Installation

Step 9: When the driver installation is complete, the screen in **Figure 6-17** appears.

Step 10: Click **FINISH** to exit setup.

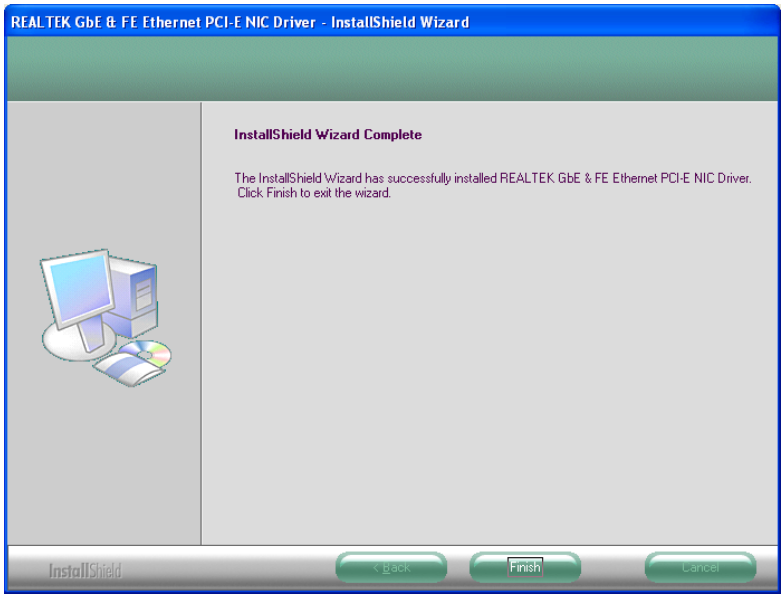
REALTEK GbE & FE Ethernet PCI-E NIC Driver - InstallShield Wizard
InstallShield Wizard Complete
The InstallShield Wizard has successfully installed REALTEK GbE & FE Ethernet PCI-E NIC Driver. Click Finish to exit the wizard.
InstallShield
< Back
Finish
Cancel

Figure 6-17: LAN Driver Installation Complete

6.5 Audio Driver Installation

To install the Realtek High Definition (HD) Audio driver, please follow the steps below.

6.5.1 BIOS Setup

Step 1: Enter the BIOS setup. To do this, reboot the system and press **F2** during POST.

Step 2: Go to the Southbridge Configuration menu. Set the **Audio Controller** option to [Azalia].

Step 3: Press **F10** to save the changes and exit the BIOS setup. The system reboots.

6.5.2 Driver Installation

To install the audio driver, please do the following.

Step 1: Access the driver list from the driver CD

Step 2: Click **Audio** then double click on the folder which corresponds to your operating system.

Step 3: Locate the install icon and double click on it.

Step 4: The **InstallShield Wizard** starts (**Figure 6-18**).

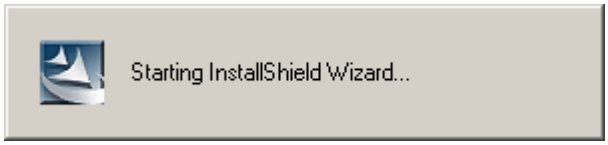

Figure 6-18: The InstallShield Wizard Starts

Step 5: The **InstallShield Wizard** is prepared to guide the user through the rest of the process (**Figure 6-19**).

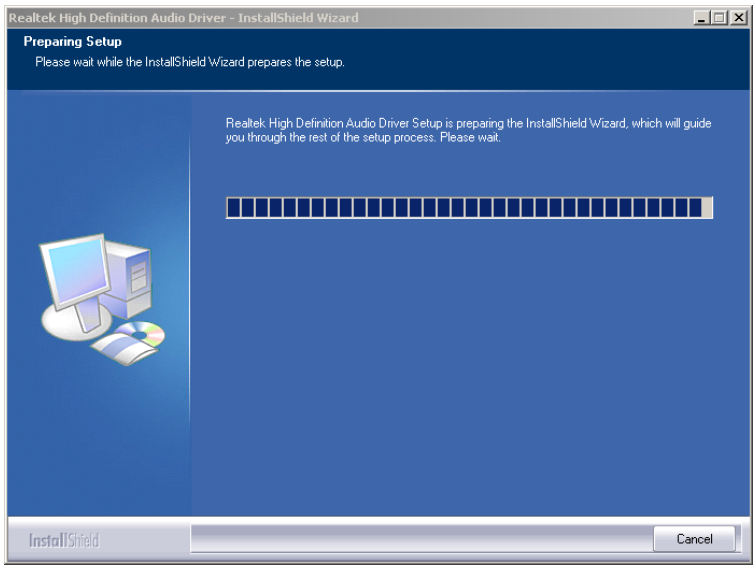
Realtek High Definition Audio Driver - InstallShield Wizard
Preparing Setup
Please wait while the InstallShield Wizard prepares the setup.
Realtek High Definition Audio Driver Setup is preparing the InstallShield Wizard, which will guide you through the rest of the setup process. Please wait.
InstallShield
Cancel

Figure 6-19: Preparing Setup Screen

Step 6: Once initialized, the **InstallShield Wizard** welcome screen appears (**Figure 6-20**).

Step 7: Click **NEXT** to continue the installation.

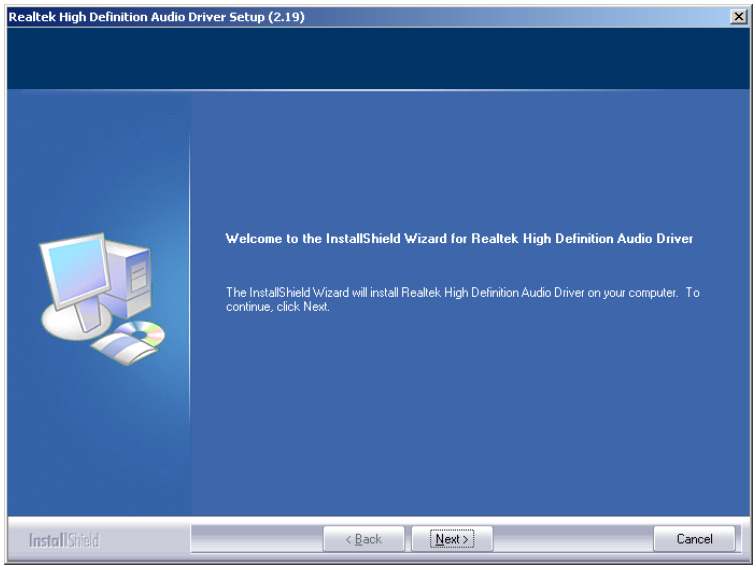
Realtek High Definition Audio Driver Setup (2.19)
Welcome to the InstallShield Wizard for Realtek High Definition Audio Driver
The InstallShield Wizard will install Realtek High Definition Audio Driver on your computer. To continue, click Next.
InstallShield
< Back
Next >
Cancel

Figure 6-20: InstallShield Wizard Welcome Screen

Step 8: InstallShield starts to install the new software as shown in **Figure 6-21**.

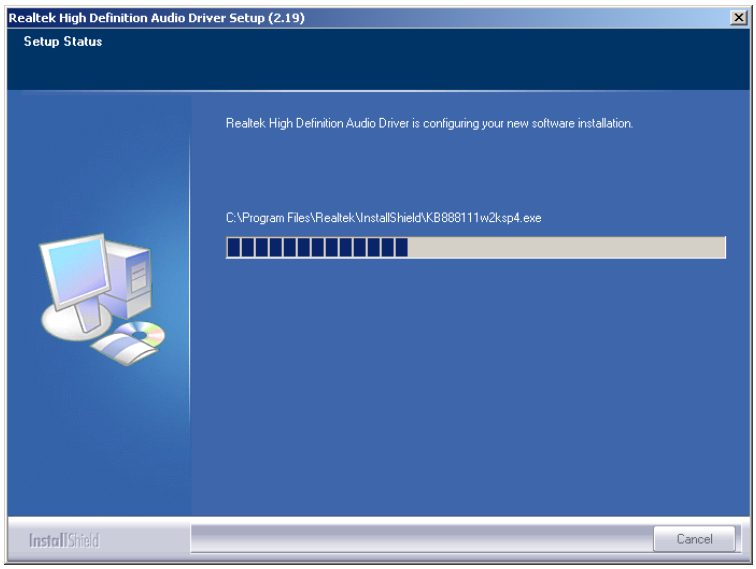
Realtek High Definition Audio Driver Setup (2.19)
Setup Status
Realtek High Definition Audio Driver is configuring your new software installation.
C:\Program Files\Realtek\InstallShield\KB888111w2ksp4.exe
InstallShield
Cancel

Figure 6-21: Audio Driver Progress Screen

Step 9: The Installation Wizard updates the system as shown in **Figure 6-22**.

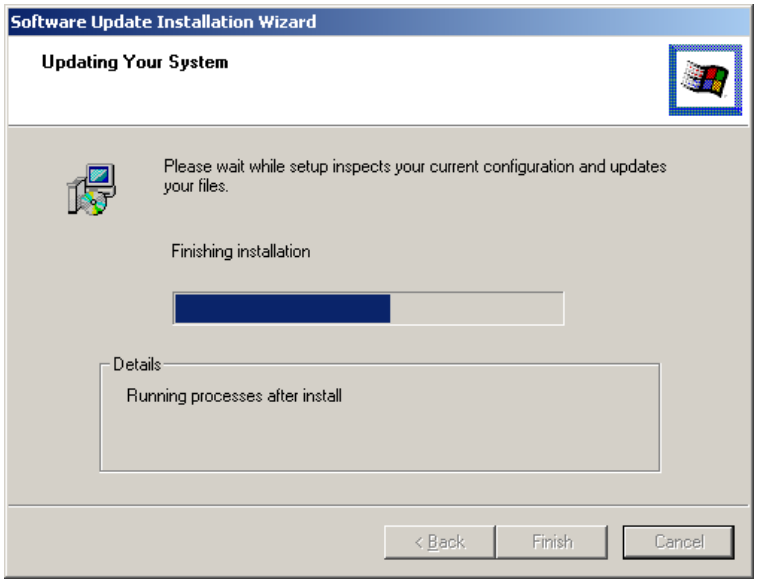

Figure 6-22: Installation Wizard Updates the System

Step 10: After the driver installation process is complete, a confirmation screen appears (**Figure 6-23**).

Step 11: The confirmation screen offers the option of restarting the computer now or later. For the settings to take effect, the computer must be restarted.

Step 12: Click **FINISH** to restart the computer.

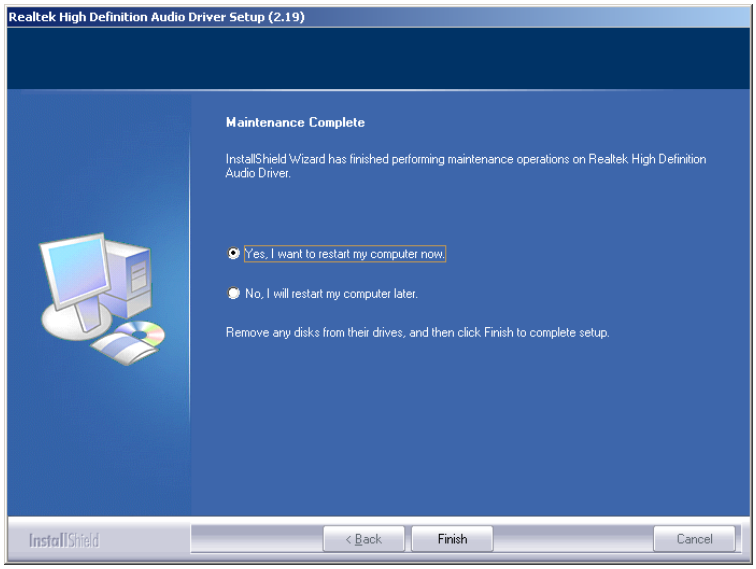
Realtek High Definition Audio Driver Setup (2.19)
Maintenance Complete
InstallShield Wizard has finished performing maintenance operations on Realtek High Definition Audio Driver.
Yes, I want to restart my computer now.
No, I will restart my computer later.
Remove any disks from their drives, and then click Finish to complete setup.
InstallShield
< Back
Finish
Cancel

Figure 6-23: Restart the Computer

6.6 Touch Screen Driver

To install the touch panel software driver, please follow the steps below.

Step 1: Access the driver list from the driver CD

Step 2: Click **Touch Screen**.

Step 3: Open the **x:\5. Touch Screen\PenMount Windows Universal Driver V2.1.0.263** directory and locate the installation icon **setup.exe**. Double click on the icon.

Step 4: The **Welcome Screen** appears (**Figure 6-24**).

Step 5: Click **NEXT** to continue the installation process.

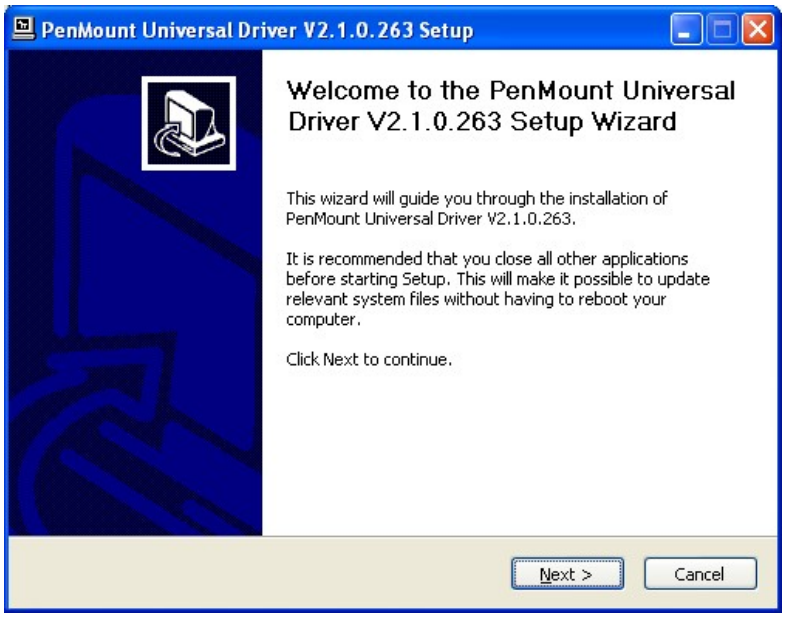
PenMount Universal Driver V2.1.0.263 Setup
Welcome to the PenMount Universal Driver V2.1.0.263 Setup Wizard
This wizard will guide you through the installation of PenMount Universal Driver V2.1.0.263.
It is recommended that you close all other applications before starting Setup. This will make it possible to update relevant system files without having to reboot your computer.
Click Next to continue.
Next >
Cancel

Figure 6-24: PenMount Welcome Screen

Step 6: The **License Agreement** shown in **Figure 6-25** appears.

Step 7: Click **I AGREE** to accept and continue.

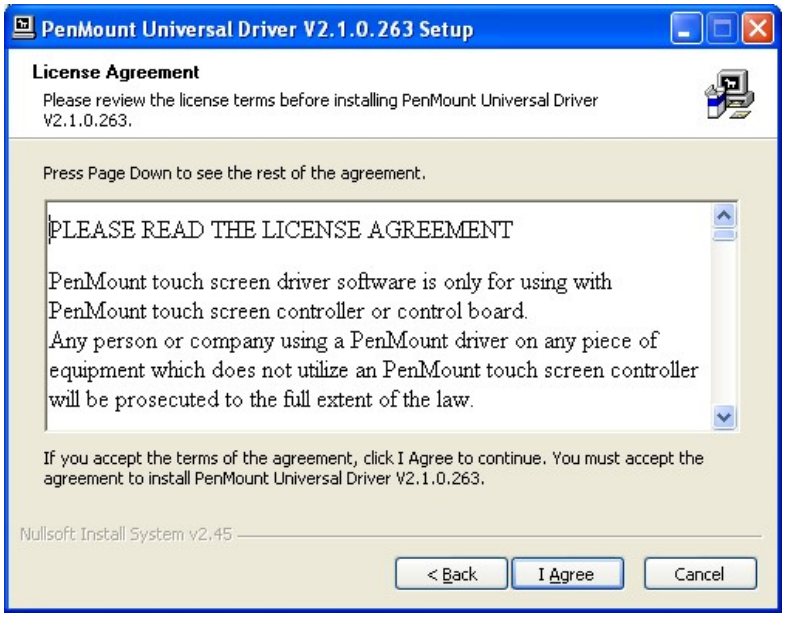
PenMount Universal Driver V2.1.0.263 Setup
License Agreement
Please review the license terms before installing PenMount Universal Driver V2.1.0.263.
Press Page Down to see the rest of the agreement.
PLEASE READ THE LICENSE AGREEMENT
PenMount touch screen driver software is only for using with PenMount touch screen controller or control board.
Any person or company using a PenMount driver on any piece of equipment which does not utilize an PenMount touch screen controller will be prosecuted to the full extent of the law.
If you accept the terms of the agreement, click I Agree to continue. You must accept the agreement to install PenMount Universal Driver V2.1.0.263.
Nullsoft Install System v2.45
< Back
I Agree
Cancel

Figure 6-25: License Agreement

Step 8: Browse for an install location or use the one suggested then click **INSTALL** to continue (Figure 6-26).

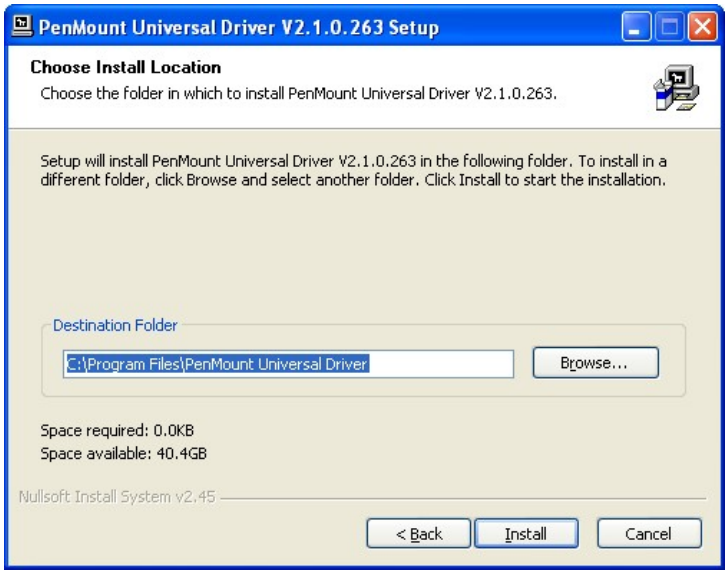
PenMount Universal Driver V2.1.0.263 Setup
Choose Install Location
Choose the folder in which to install PenMount Universal Driver V2.1.0.263.
Setup will install PenMount Universal Driver V2.1.0.263 in the following folder. To install in a different folder, click Browse and select another folder. Click Install to start the installation.
Destination Folder
C:\Program Files\PenMount Universal Driver
Browse...
Space required: 0.0KB
Space available: 40.4GB
Nullsoft Install System v2.45
< Back
Install
Cancel

Figure 6-26: Choose Install Location

Step 9: The **Install** screen appears and displays the progress of the installation (Figure 6-27). Click **NEXT** to continue.

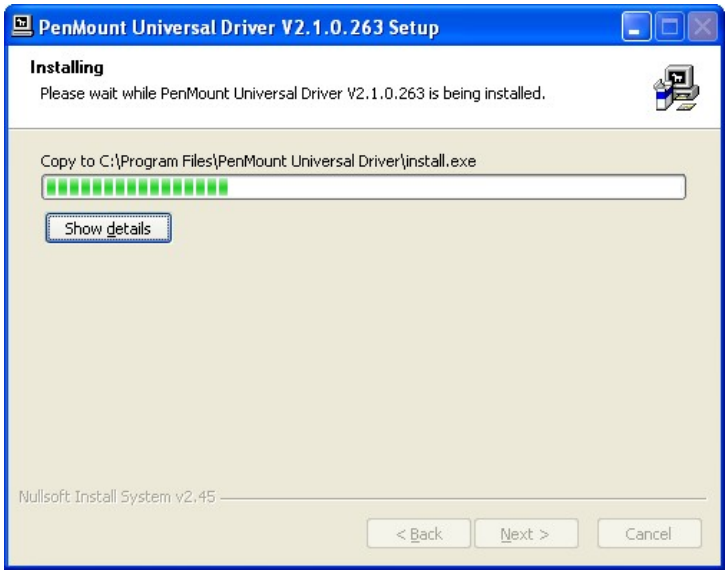
PenMount Universal Driver V2.1.0.263 Setup
Installing
Please wait while PenMount Universal Driver V2.1.0.263 is being installed.
Copy to C:\Program Files\PenMount Universal Driver\install.exe
Show details
Nullsoft Install System v2.45
< Back
Next >
Cancel

Figure 6-27: Installing PenMount Universal Driver V2.1.0.263

Step 10: When the installation is complete, click **FINISH** to exit setup (Figure 6-28).

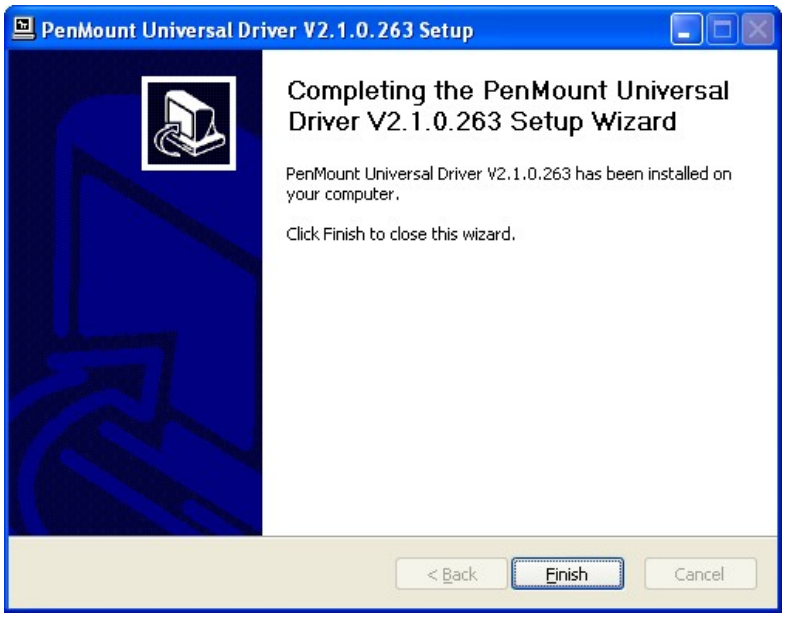
PenMount Universal Driver V2.1.0.263 Setup
Completing the PenMount Universal Driver V2.1.0.263 Setup Wizard
PenMount Universal Driver V2.1.0.263 has been installed on your computer.
Click Finish to close this wizard.
< Back
Finish
Cancel

Figure 6-28: PenMount Universal Driver Update Complete

6.7 Wireless Driver

To install the wireless driver, please follow the steps below.

Step 1: Select **Wireless** from the list from the driver CD

Step 2: Select an OS folder then double click the installation icon **setup.exe**.

Step 3: The license agreement in **Figure 6-29** appears.

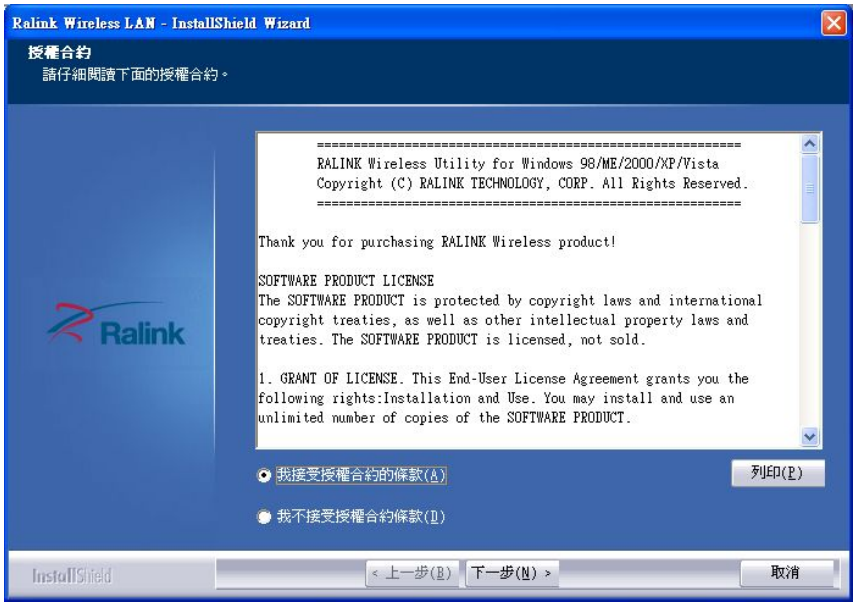
Ralink Wireless LAN - InstallShield Wizard
授權合約
請仔細閱讀下面的授權合約。
RALINK Wireless Utility for Windows 98/ME/2000/XP/Vista
Copyright (C) RALINK TECHNOLOGY, CORP. All Rights Reserved.
Thank you for purchasing RALINK Wireless product!
SOFTWARE PRODUCT LICENSE
The SOFTWARE PRODUCT is protected by copyright laws and international copyright treaties, as well as other intellectual property laws and treaties. The SOFTWARE PRODUCT is licensed, not sold.
1. GRANT OF LICENSE. This End-User License Agreement grants you the following rights:Installation and Use. You may install and use an unlimited number of copies of the SOFTWARE PRODUCT.
我接受授權合約的條款(A)
我不接受授權合約條款(D)
列印(P)
Ralink
InstallShield
< 上一步(B)
下一步(N) >
取消

Figure 6-29: Wireless Driver License Agreement

Step 4: Accept the conditions of the license agreement and click **NEXT** to continue.

Step 5: The **Configuration Tool Options** screen in **Figure 6-30** appears next.

Step 6: Select the configuration tool in and click **NEXT** to continue.

Figure 6-30: Wireless Driver Configuration Tool Options

Step 7: The **Wireless Mode Options** window in **Figure 6-31** appears.

Step 8: Click **NEXT** in **Figure 6-31**.

Figure 6-31: Wireless Mode Select Window

Step 9: Click **INSTALL** in **Figure 6-32** to start to install the driver.

Figure 6-32: Wireless Driver Installation

Step 10: After the installation is complete, click **FINISH** to exit setup.

6.8 Keypad Driver

To install the Keypad software driver, please follow the steps below.

Step 1: Select **Keypad** from the list from the driver CD

Step 2: Locate the installation icon "**KeypadAP_v2.2.msi**" and double click on it.

Step 3: The **Welcome Screen** appears (**Figure 6-33**).

Step 4: Click **NEXT** to continue the installation process.

KeypadAP v2.2 - InstallShield Wizard
Welcome to the InstallShield Wizard for KeypadAP v2.2
The InstallShield(R) Wizard will install KeypadAP v2.2 on your computer. To continue, click Next.
WARNING: This program is protected by copyright law and international treaties.
< Back
Next >
Cancel

Figure 6-33: Keypad Driver Welcome Screen

Step 5: The **Customer Information** appears as shown in **Figure 6-34**.

Step 6: Enter user and organization name in the fields provided then click **NEXT**.

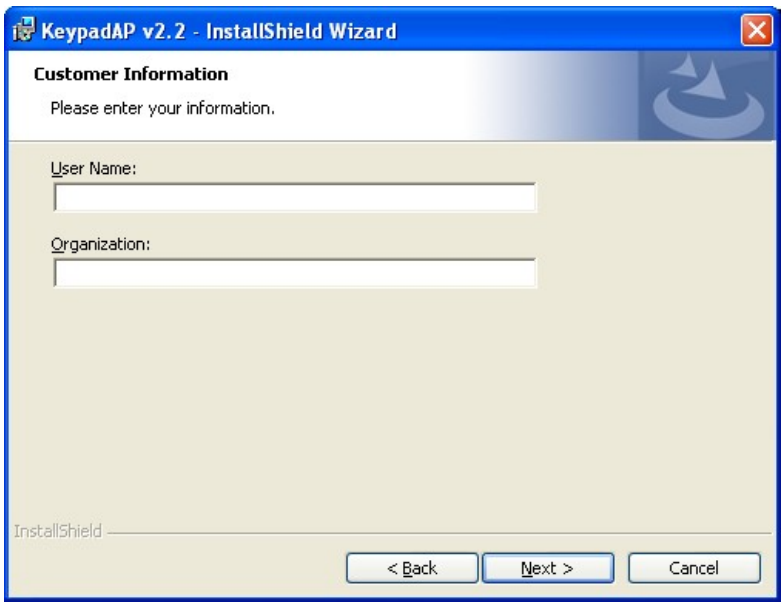

Figure 6-34: Customer Information Screen

Step 7: Select a setup type (**Figure 6-35**) and click **NEXT**.

KeypadAP v2.2 - InstallShield Wizard
Setup Type
Choose the setup type that best suits your needs.
Please select a setup type.
Complete
All program features will be installed. (Requires the most disk space.)
Custom
Choose which program features you want installed and where they will be installed. Recommended for advanced users.
InstallShield
< Back
Next >
Cancel

Figure 6-35: Setup Type

Step 8: The InstallShield Wizard is ready to install the program.

Step 9: Click **INSTALL** to continue (**Figure 6-36**).

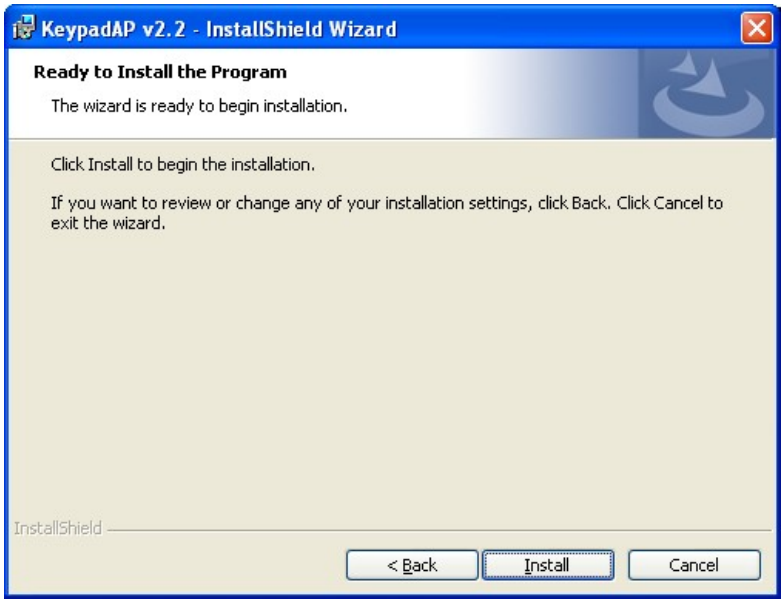
KeypadAP v2.2 - InstallShield Wizard
Ready to Install the Program
The wizard is ready to begin installation.
Click Install to begin the installation.
If you want to review or change any of your installation settings, click Back. Click Cancel to exit the wizard.
InstallShield
< Back
Install
Cancel

Figure 6-36: Ready to Install the Program

Step 10: The installation screen appears and displays the progress of the installation (**Figure 6-37**).

Step 11: Click **NEXT** to continue.

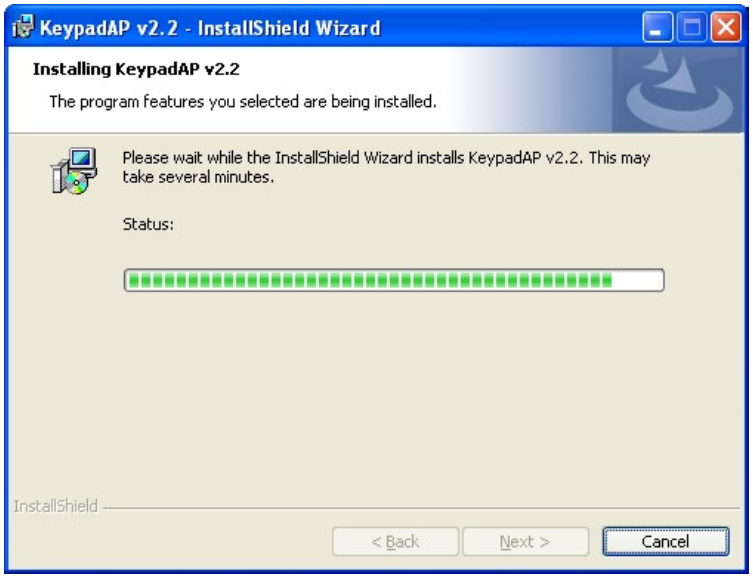
KeypadAP v2.2 - InstallShield Wizard
Installing KeypadAP v2.2
The program features you selected are being installed.
Please wait while the InstallShield Wizard installs KeypadAP v2.2. This may take several minutes.
Status:
InstallShield
< Back
Next >
Cancel

Figure 6-37: Installing KeypadAP v2.2

Step 12: When the installation process is complete, click **FINISH**. See **Figure 6-38**.

KeypadAP v2.2 - InstallShield Wizard
InstallShield Wizard Completed
The InstallShield Wizard has successfully installed KeypadAP v2.2. Click Finish to exit the wizard.
< Back
Finish
Cancel

Figure 6-38: Keypad Driver Installation Complete Screen

Step 13: The user is then prompted to select to restart the computer now or later (**Figure 6-47**). For the settings to take effect, the computer must be restarted.

Step 14: Click **Yes** to restart the computer.

KeypadAP v2.2 Installer Information
You must restart your system for the configuration changes made to KeypadAP v2.2 to take effect. Click Yes to restart now or No if you plan to restart later.
Yes
No

Figure 6-39: Reboot the Computer

Appendix

A

Safety Precautions

WARNING:

The precautions outlined in this chapter should be strictly followed. Failure to follow these precautions may result in permanent damage to the POC-17i/19i Series.

A.1 Safety Precautions

Please follow the safety precautions outlined in the sections that follow:

A.1.1 General Safety Precautions

Please ensure the following safety precautions are adhered to at all times.

- ***Follow the electrostatic precautions*** outlined below whenever the system is opened.
- ***Make sure the power is turned off and the power cord is disconnected*** whenever the system is being installed, moved or modified.
- ***Do not apply voltage levels that exceed the specified voltage range***. Doing so may cause fire and/or an electrical shock.
- ***Use a power cord that matches the voltage of the power outlet***, which has been approved and complies with the safety standard of your particular country.
- ***Electric shocks can occur*** if the system chassis is opened when the system is running.
- ***Do not drop or insert any objects*** into the ventilation openings of the system.
- ***If considerable amounts of dust, water, or fluids enter the system***, turn off the power supply immediately, unplug the power cord, and contact the system vendor.
- Grounding reliability can only be achieved when the equipment is connected to an equivalent receptacle marked “Hospital Only” or “Hospital Grade”.

- The signal input parts or signal output parts (SIP/SOP) need to be connected properly and any unused SIP/SOP shall not be accessible to unqualified personnel after the LCD is integrated into a medical system.
- The unit is for exclusive interconnection with IEC 60XXX certified equipment outside of patient environment and IEC 60601-1 certified equipment inside the patient environment.
- This device complies with EN60601-1-2. To minimize the interference from other equipment, a minimum 0.5 m distance shall be kept from other potential electromagnetic sources, such as cell phones, etc.
- Equipment connected to the analog or digital interfaces must comply with the respective IEC standards (e.g. IEC 60950 for data processing equipment and IEC 60601-1 for medical equipment).
- **Caution** – Use suitable mounting apparatus to avoid risk of injury.
- **Warning** – Do not modify this equipment without authorization of the manufacturer.
- **Warning** – To avoid risk of electric shock, this equipment must only be connected to a supply mains with protective earth. Instructions provided indicating not to position ME EQUIPMENT to make it difficult to operate the disconnection device when an appliance coupler or separable plug is used as isolation means to meet Chapter 3.1).
- **Caution** – This adapter FSP Group Inc. PMP120-12-S is a forming part of the medical device.
- Make sure the user not to contact SIP/SOPs and the patient at the same time.
- **DO NOT**:
  - Drop the system against a hard surface.
  - Strike or exert excessive force onto the LCD panel.
  - Touch any of the LCD panels with a sharp object
  - In a site where the ambient temperature exceeds the rated temperature

A.1.2 Explanation of Graphical Symbols

This symbol warns the user that uninsulated voltage within the unit may have sufficient magnitude to cause electric shock. Therefore, it is dangerous to make any kind of contact with any part inside this unit.

This symbol alerts the user that important information concerning the operation and maintenance of this unit has been included. Therefore, the information should be read carefully in order to avoid any problems.

ISO 7000-1641: Follow operating instructions or consult instructions for use.

Stand-by

Direct Current

A.1.3 Anti-static Precautions

WARNING:

Failure to take ESD precautions during the installation of the system may result in permanent damage to the system and severe injury to the user.

Electrostatic discharge (ESD) can cause serious damage to electronic components, including the system. Dry climates are especially susceptible to ESD. It is therefore critical that whenever the system is opened and any of the electrical components are handled, the following anti-static precautions are strictly adhered to.

- ***Wear an anti-static wristband***: Wearing a simple anti-static wristband can help to prevent ESD from damaging any electrical component.
- ***Self-grounding***: Before handling any electrical component, touch any grounded conducting material. During the time the electrical component is handled, frequently touch any conducting materials that are connected to the ground.
- ***Use an anti-static pad***: When configuring or working with an electrical component, place it on an antic-static pad. This reduces the possibility of ESD damage.
- ***Only handle the edges of the electrical component***: When handling the electrical component, hold the electrical component by its edges.

A.1.4 Product Disposal

- Outside the European Union - If you wish to dispose of used electrical and electronic products outside the European Union, please contact your local authority so as to comply with the correct disposal method.
- Within the European Union:



EU-wide legislation, as implemented in each Member State, requires that waste electrical and electronic products carrying the mark (left) must be disposed of separately from normal household waste. This includes monitors and electrical accessories, such as signal cables or power cords. When you need to dispose of your display products, please follow the guidance of your local authority, or ask the shop where you purchased the product. The mark on electrical and electronic products only applies to the current European Union Member States.

Please follow the national guidelines for electrical and electronic product disposal.

A.2 Maintenance and Cleaning Precautions

When maintaining or cleaning the system, please follow the guidelines below.

A.2.1 Maintenance and Cleaning

Prior to cleaning any part or component of the system, please read the details below.

- Special maintenance is not necessary during normal use of the POC-17i/19i Series panel PC. If the user has any questions on how to operate the panel PC, please contact the manufacturer for technical support and customer service (contact information is listed on Page iv).
- Parts requiring preventive inspection and maintenance to be performed by service personnel identified including periods of application.
- Except for the LCD panel, never spray or squirt liquids directly onto any other components. To clean the LCD panel, gently wipe it with a piece of soft dry cloth or a slightly moistened cloth.
- The interior of the system does not require cleaning. Keep fluids away from the system interior.

- Be cautious of all small removable components when vacuuming the system.
- Turn the system off before cleaning the system.
- Never drop any objects or liquids through the openings of the system.
- Avoid eating, drinking and smoking within vicinity of the system.

A.2.2 Cleaning Tools

Some components in the system may only be cleaned using a product specifically designed for the purpose. In such case, the product will be explicitly mentioned in the cleaning tips. Below is a list of items to use when cleaning the system.

- ***Cloth*** – Although paper towels or tissues can be used, a soft, clean piece of cloth is recommended when cleaning the system.
- ***Vacuum cleaner*** – Using a vacuum specifically designed for computers is one of the best methods of cleaning the system. Dust and dirt can restrict the airflow in the system and cause its circuitry to corrode.

A.3 FCC Precautions

WARNING:

This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.

- Consult the dealer or an experienced radio/TV technician for help.

FCC Caution: Any changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate this equipment.

This device and its antenna(s) must not be co-located or operating in conjunction with any other antenna or transmitter.

IMPORTANT NOTE:

For product available in the USA/Canada market, only channel 1~11 can be operated. Selection of other channels is not possible.

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Appendix

B

BIOS Options

B.1 BIOS Configuration Options

Below is a list of BIOS configuration options described in **Chapter 5**.

System Overview **52**
Memory Information **52**
System Date [xx/xx/xx] **53**
System Time [xx:xx:xx] **53**
ACPI Sleep State [S3 (CPU Stop Clock)] **55**
TPM Support [Disable] **56**
SATA Mode [IDE Mode] **57**
Serial-ATA Controller n [Compatible] **57**
USB Devices **58**
All USB Devices [Enabled] **58**
Legacy USB Support [Enabled] **59**
Serial Port [Enabled] **60**
Change Settings [Auto] **60**
Serial Port [Enabled] **61**
Change Settings [Auto] **61**
Serial Port [Enabled] **62**
Change Settings [Auto] **62**
Parallel Port [Enabled] **63**
Change Settings [Auto] **63**
Device Mode [Printer Mode] **63**
PC Health Status **64**
Console Redirection [Disabled] **65**
IGD Memory [32 MB] **67**
Restore on AC Power Loss [Power Off] **68**
Azalia HD Audio [Enabled] **68**
Set Spread Spectrum [Disabled] **69**
DVMT/FIXED Memory [Maximum] **69**
Active LFP [Enable LVDS] **70**
LCD Panel Type [Select by Panel ID] **70**
Quiet Boot [Enabled] **71**
Bootup NumLock State [On] **71**

Realtek 8111E PXE OpROM [Disabled].....72
Administrator Password 73
User Password 73
Set User Password 73
Save Changes and Reset 74
Discard Changes and Reset 74
Restore Defaults 74
Save as User Defaults 74
Restore User Defaults 74

Appendix

C

Watchdog Timer

NOTE:

The following discussion applies to DOS environment. PACSmate support is contacted or the PACSmate website visited for specific drivers for more sophisticated operating systems, e.g., Windows and Linux.

The Watchdog Timer is provided to ensure that standalone systems can always recover from catastrophic conditions that cause the CPU to crash. This condition may have occurred by external EMI or a software bug. When the CPU stops working correctly, Watchdog Timer either performs a hardware reset (cold boot) or a Non-Maskable Interrupt (NMI) to bring the system back to a known state.

A BIOS function call (INT 15H) is used to control the Watchdog Timer:

INT 15H:

AH – 6FH Sub-function:	
AL – 2:	Sets the Watchdog Timer's period.
BL:	Time-out value (Its unit-second is dependent on the item "Watchdog Timer unit select" in CMOS setup).

Table C-1: AH-6FH Sub-function

Call sub-function 2 to set the time-out period of Watchdog Timer first. If the time-out value is not zero, the Watchdog Timer starts counting down. While the timer value reaches zero, the system resets. To ensure that this reset condition does not occur, the calling sub-function 2 must periodically refresh the Watchdog Timer. However, the Watchdog timer is disabled if the time-out value is set to zero.

A tolerance of at least 10% must be maintained to avoid unknown routines within the operating system (DOS), such as disk I/O that can be very time-consuming.

NOTE:

When exiting a program it is necessary to disable the Watchdog Timer, otherwise the system resets.

Example program:

```
; INITIAL TIMER PERIOD COUNTER
;
W_LOOP:

        MOV     AX, 6F02H     ;setting the time-out value
        MOV     BX, 05        ;time-out value is 5 seconds
        INT      15H
 ;
; ADD THE APPLICATION PROGRAM HERE
;
        CMP      EXIT_AP, 1   ;is the application over?
        JNE      W_LOOP       ;No, restart the application

        MOV     AX, 6F02H     ;disable Watchdog Timer
        MOV     BX, 0         ;
        INT      15H
;
; EXIT ;
```

Appendix

D

Hazardous Materials Disclosure

D.1 Hazardous Material Disclosure Table for IPB Products Certified as RoHS Compliant Under 2002/95/EC Without Mercury

The details provided in this appendix are to ensure that the product is compliant with the Peoples Republic of China (China) RoHS standards. The table below acknowledges the presences of small quantities of certain materials in the product, and is applicable to China RoHS only.

A label will be placed on each product to indicate the estimated “Environmentally Friendly Use Period” (EFUP). This is an estimate of the number of years that these substances would “not leak out or undergo abrupt change.” This product may contain replaceable sub-assemblies/components which have a shorter EFUP such as batteries and lamps. These components will be separately marked.

Please refer to the table on the next page.

Part Name	Toxic or Hazardous Substances and Elements					
	Lead (Pb)	Mercury (Hg)	Cadmium (Cd)	Hexavalent Chromium (CR(VI))	Polybrominated Biphenyls (PBB)	Polybrominated Diphenyl Ethers (PBDE)
Housing	X	O	O	O	O	X
Display	X	O	O	O	O	X
Printed Circuit Board	X	O	O	O	O	X
Metal Fasteners	X	O	O	O	O	O
Cable Assembly	X	O	O	O	O	X
Fan Assembly	X	O	O	O	O	X
Power Supply Assemblies	X	O	O	O	O	X
Battery	O	O	O	O	O	O

O: This toxic or hazardous substance is contained in all of the homogeneous materials for the part is below the limit requirement in SJ/T11363-2006

X: This toxic or hazardous substance is contained in at least one of the homogeneous materials for this part is above the limit requirement in SJ/T11363-2006

此附件旨在确保本产品符合中国 RoHS 标准。以下表格标示此产品中某有毒物质的含量符合中国 RoHS 标准规定的限量要求。

本产品上会附有"环境友好使用期限"的标签，此期限是估算这些物质"不会有泄漏或突变"的年限。本产品可能包含有较短的环境友好使用期限的可替换元件，像是电池或灯管，这些元件将会单独标示出来。

部件名称	有毒有害物质或元素					
	铅 (Pb)	汞 (Hg)	镉 (Cd)	六价铬 (CR(VI))	多溴联苯 (PBB)	多溴二苯醚 (PBDE)
壳体	X	O	O	O	O	X
显示	X	O	O	O	O	X
印刷电路板	X	O	O	O	O	X
金属螺帽	X	O	O	O	O	O
电缆组装	X	O	O	O	O	X
风扇组装	X	O	O	O	O	X
电力供应组装	X	O	O	O	O	X
电池	O	O	O	O	O	O

O: 表示该有毒有害物质在该部件所有物质材料中的含量均在 SJ/T11363-2006 标准规定的限量要求以下。

X: 表示该有毒有害物质至少在该部件的某一均质材料中的含量超出 SJ/T11363-2006 标准规定的限量要求。